



30kV ESD x885 D=7.9mm P=1.0T
Centre for Microscopy, UWA 98.08.26 20:19 P

9838A07S.TIF

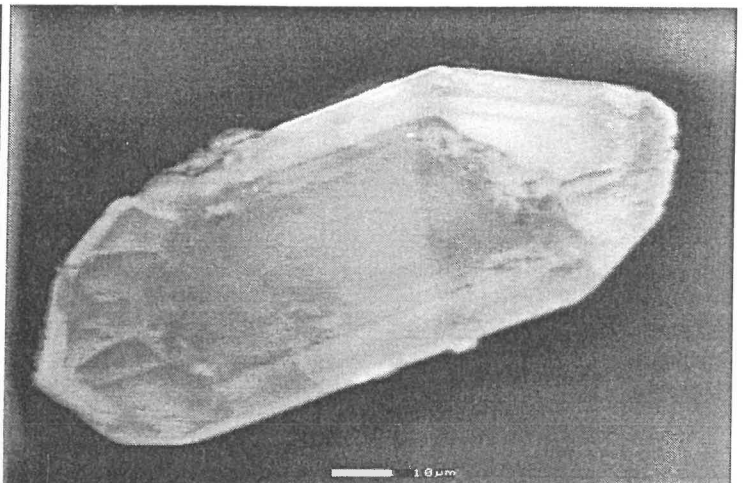


30kV ESD x1000 D=7.9mm P=1.1T
Centre for Microscopy, UWA 98.08.26 20:22 P

9838A08S.TIF

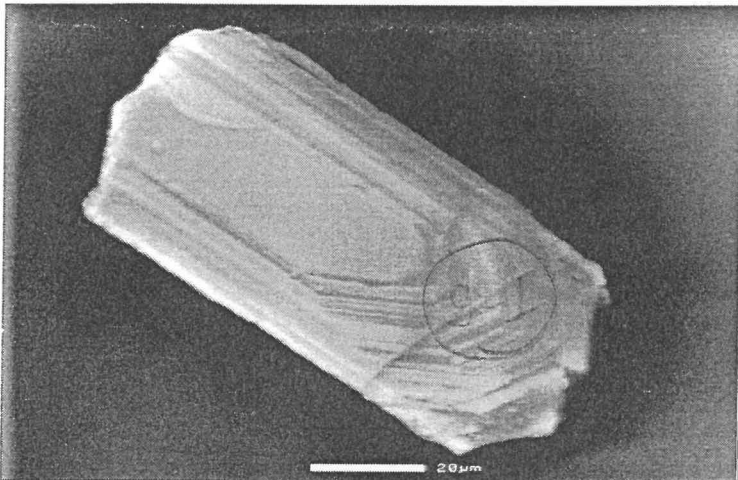


30kV ESD x990 D=7.9mm P=1.0T
Centre for Microscopy, UWA 98.08.26 20:24 P

9838A09S.TIF

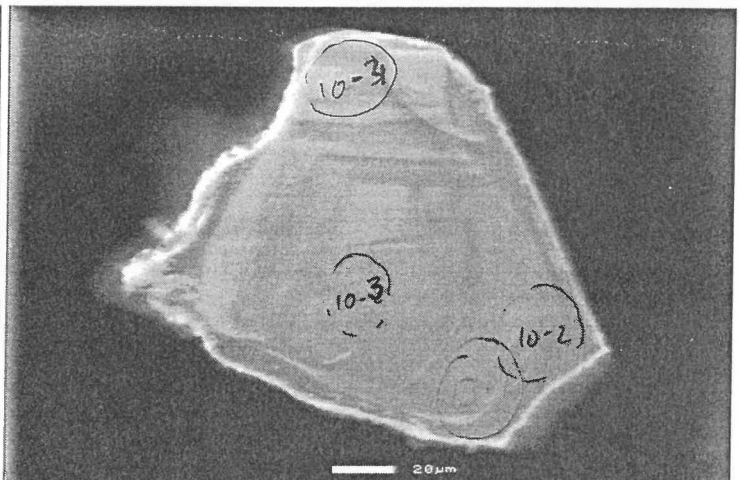


30kV ESD x520 D=7.9mm P=1.2T
Centre for Microscopy, UWA 98.08.26 20:28 P

9838A10S.TIF

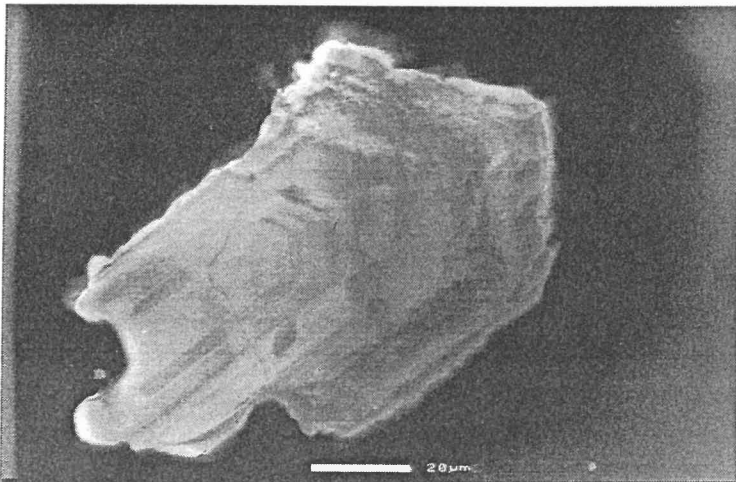







30kV ESD x855 D=7.9mm P=1.0T
Centre for Microscopy, UWA 98.08.26 20:31 P


9838A11S.TIF

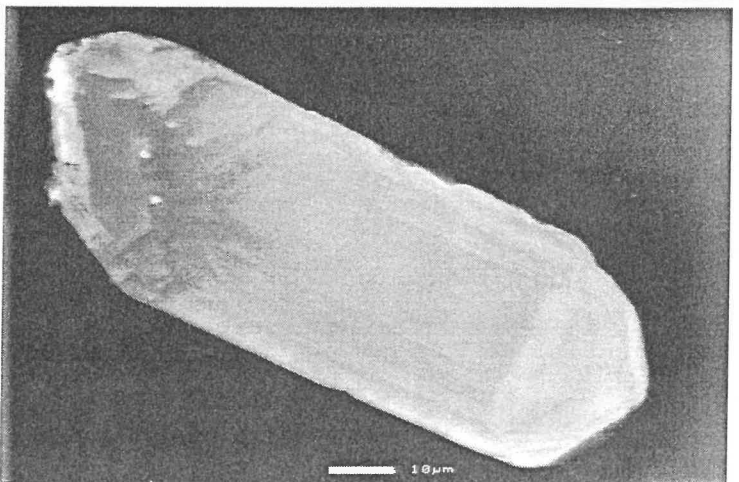

30kV ESD x1100 D=7.9mm P=1.2T
Centre for Microscopy, UWA 98.08.26 20:33 P


9838A12S.TIF

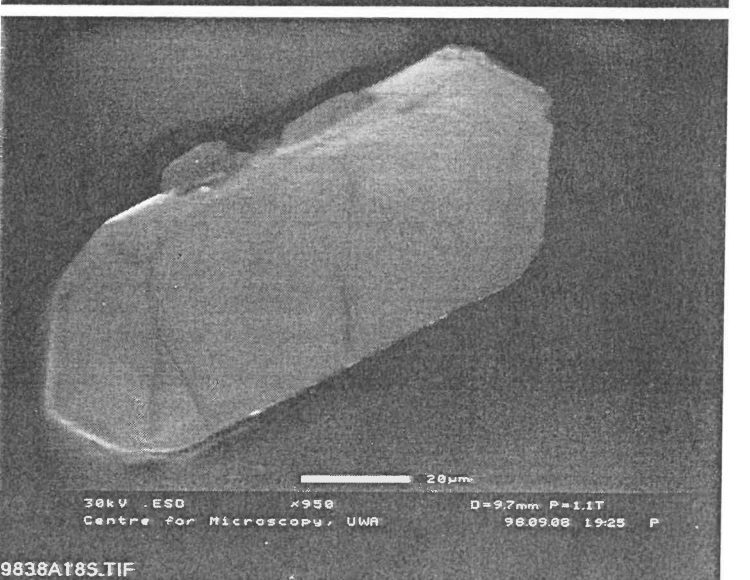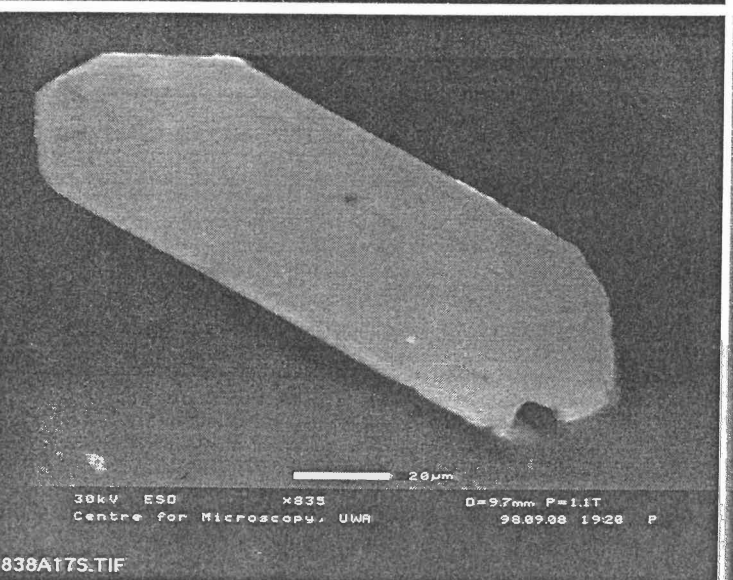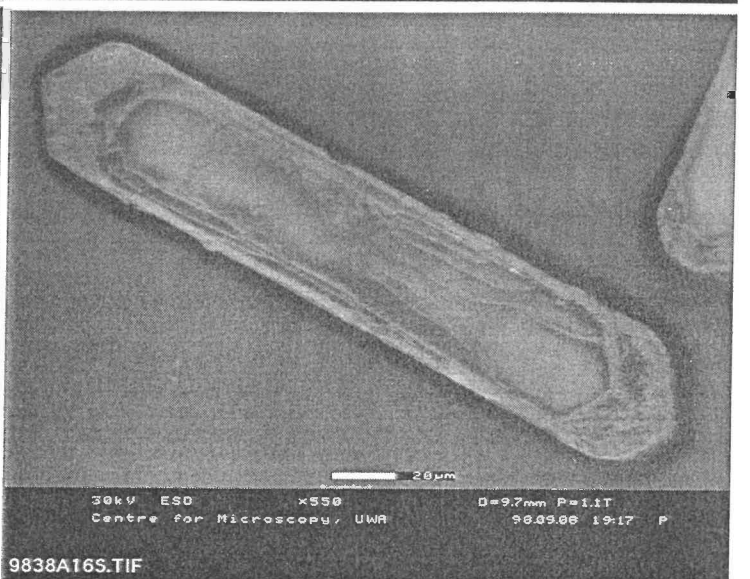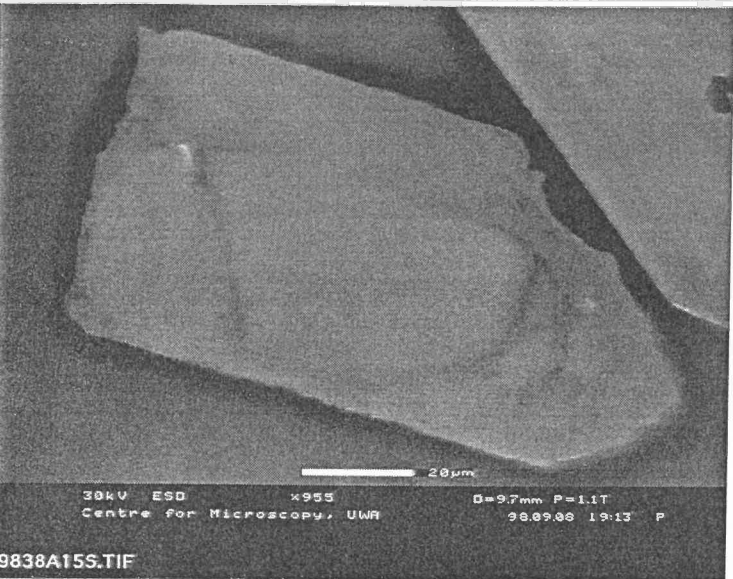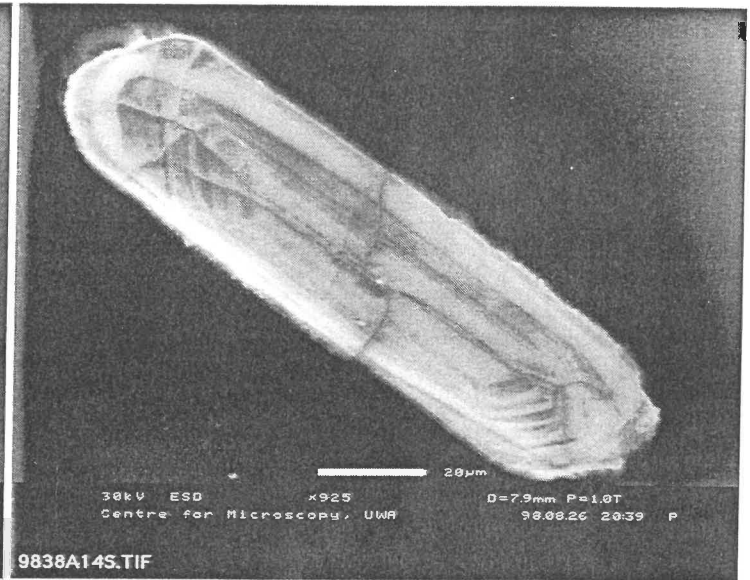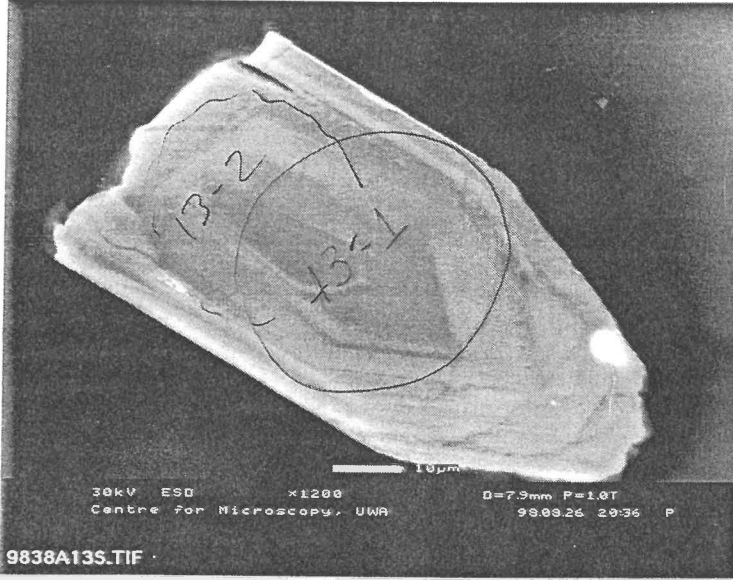

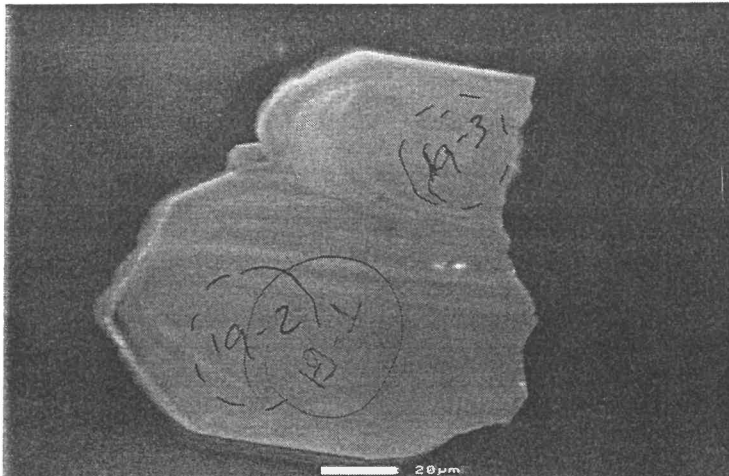


30kV ESD x630 D=9.7mm P=1.1T
Centre for Microscopy, UWA 98.09.08 19:30 P

9838A19S.TIF

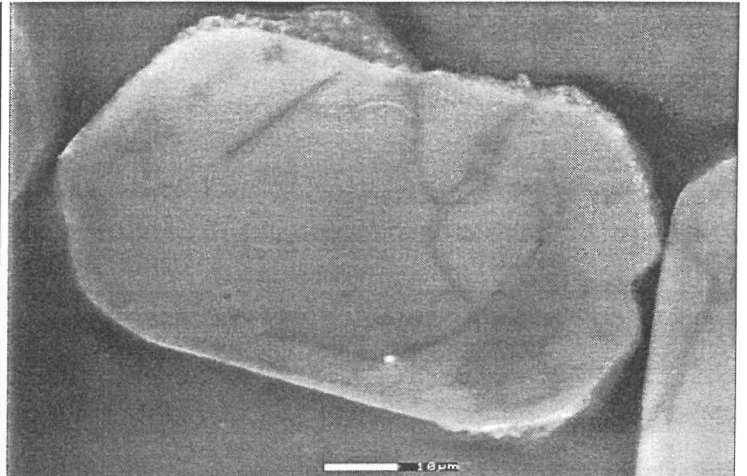


30kV ESD x1300 D=9.7mm P=1.1T
Centre for Microscopy, UWA 98.09.08 19:35 P

9838A20S.TIF

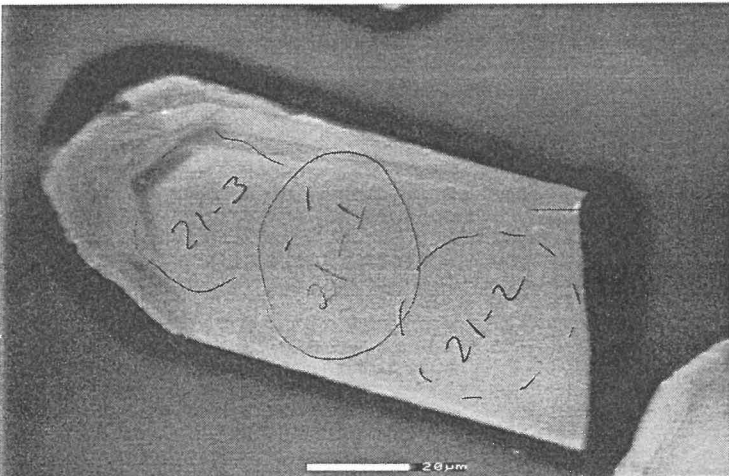


30kV ESD x800 D=9.7mm P=1.1T
Centre for Microscopy, UWA 98.09.08 19:39 P

9838A21S.TIF

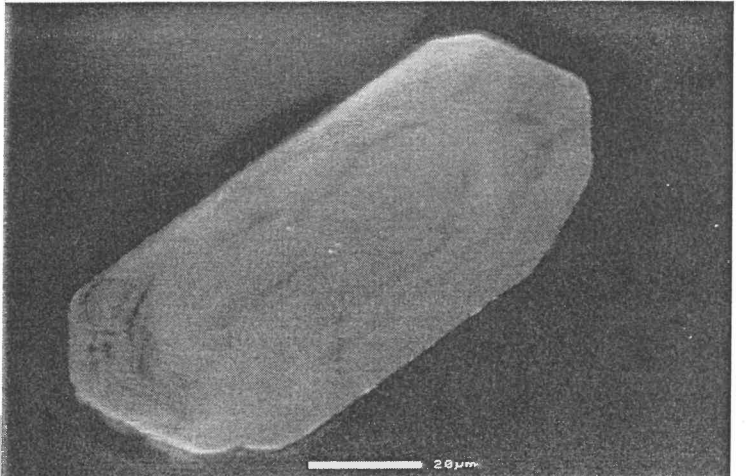


30kV ESD x985 D=9.7mm P=1.1T
Centre for Microscopy, UWA 98.09.08 19:42 P

9838A22S.TIF

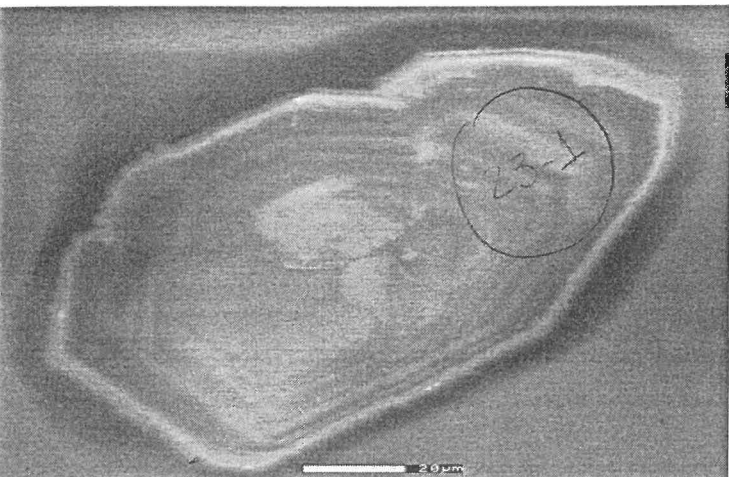







30kV ESD x875 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.08 19:48 P


9838A23S.TIF

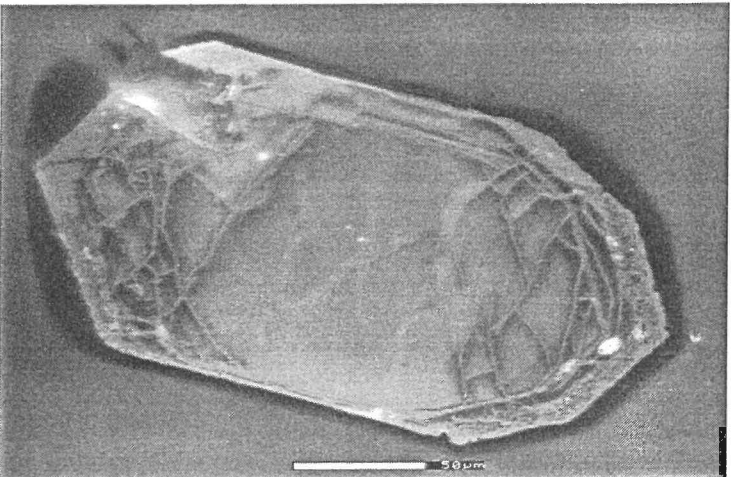

30kV ESD x460 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.08 19:58 P


9838A24S.TIF

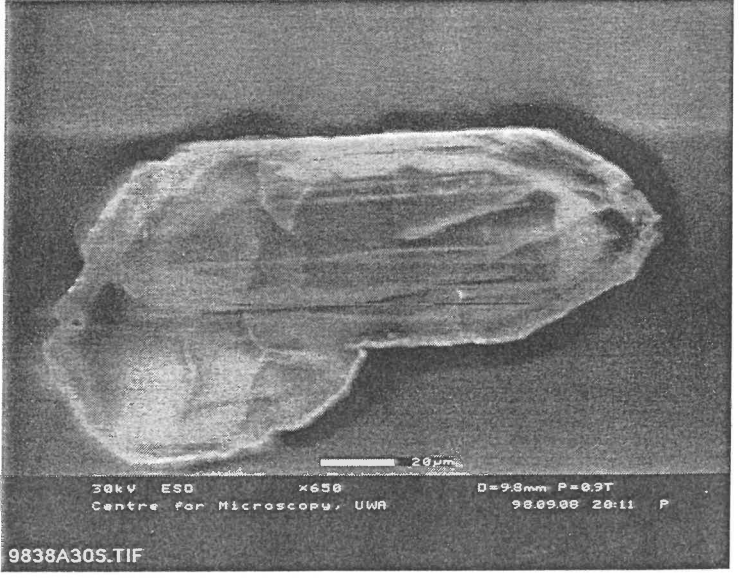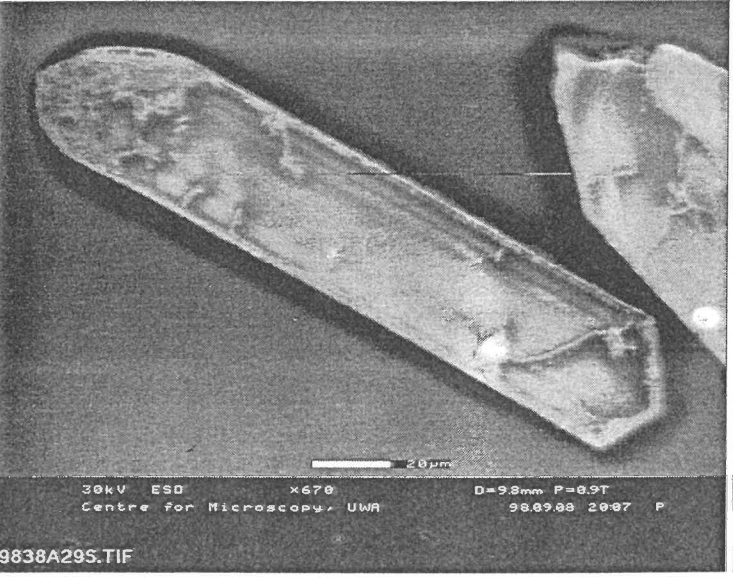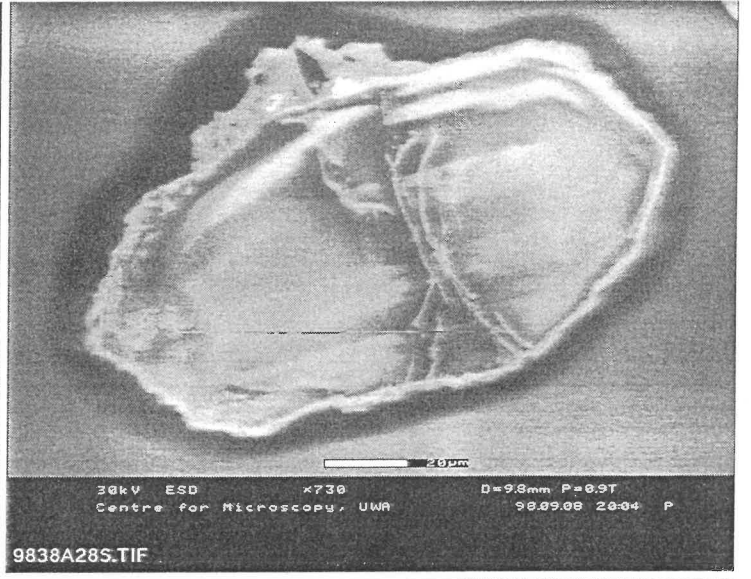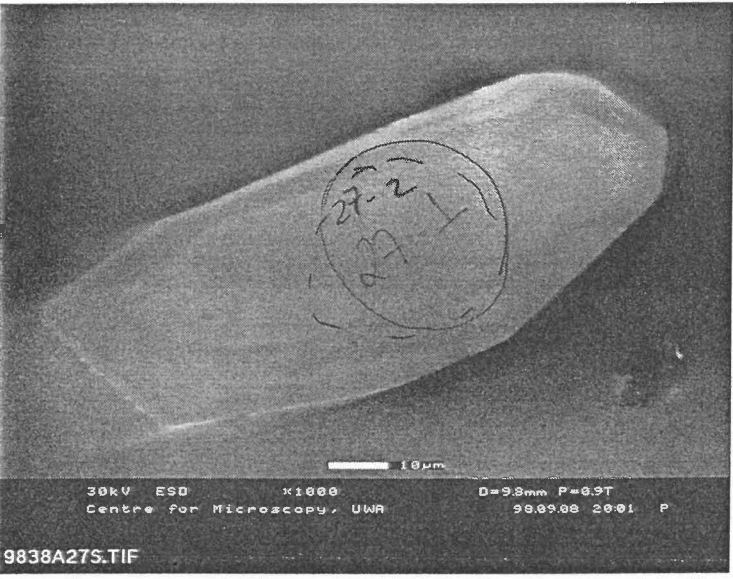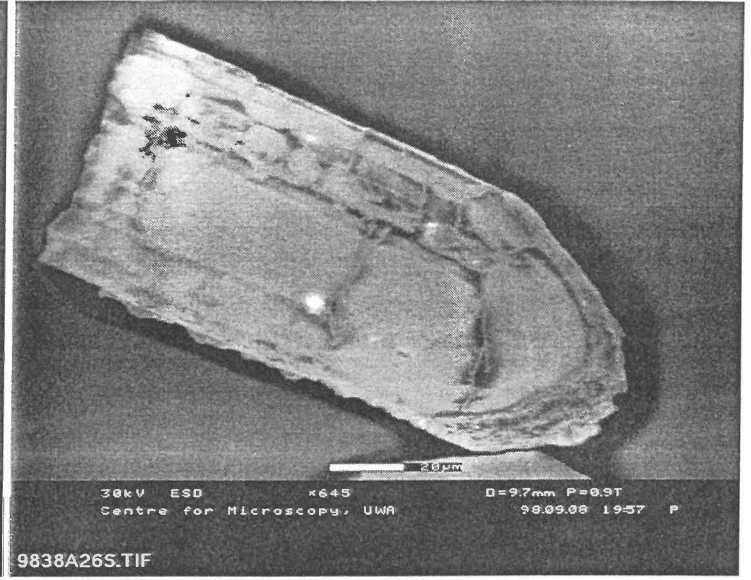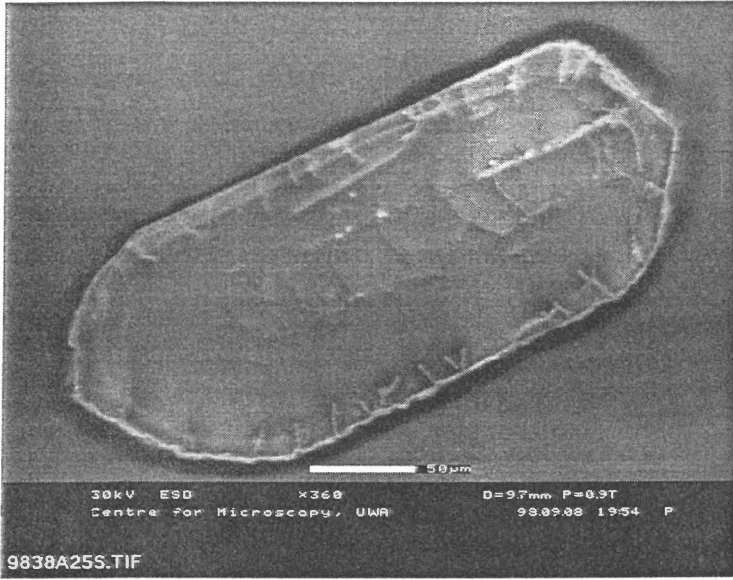

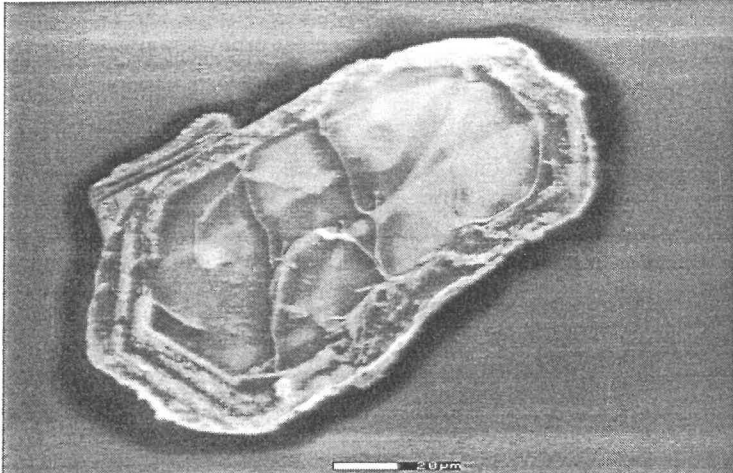


30kV ESD x535 D=9.8mm P=0.9T
Centre for Microscopy, UWA 98.09.98 20:15 P

9838A31S.TIF

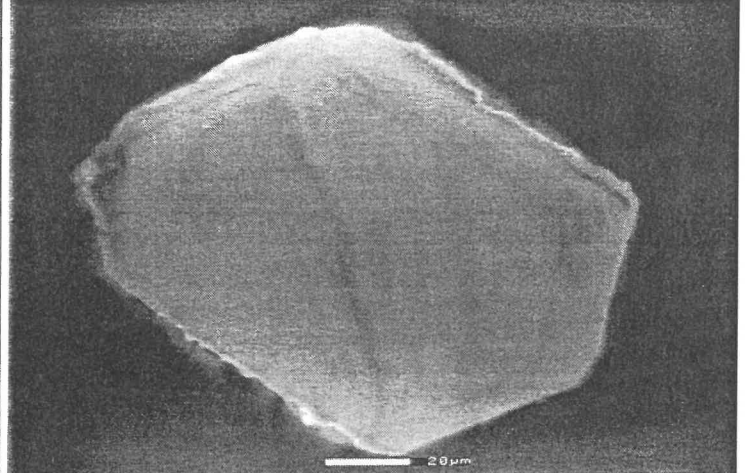


30kV ESD x735 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.98 20:18 P

9838A32S.TIF

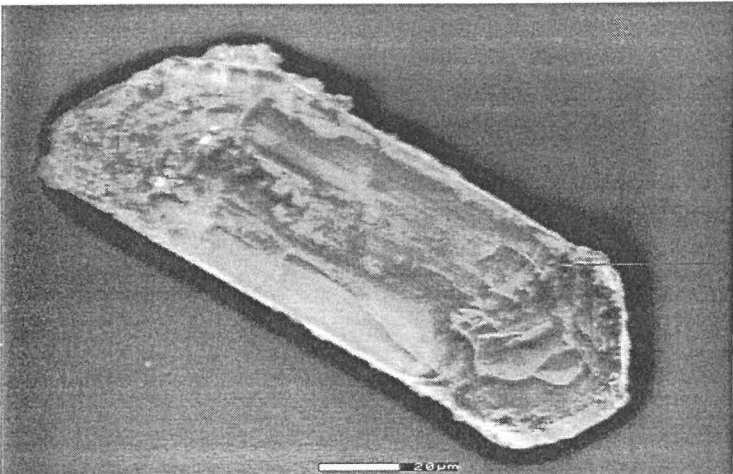


30kV ESD x680 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.98 20:20 P

9838A33S.TIF

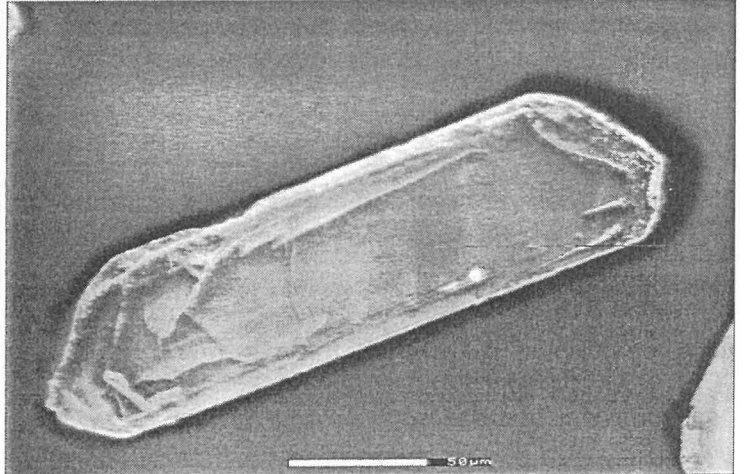


30kV ESD x485 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.98 20:23 P

9838A34S.TIF

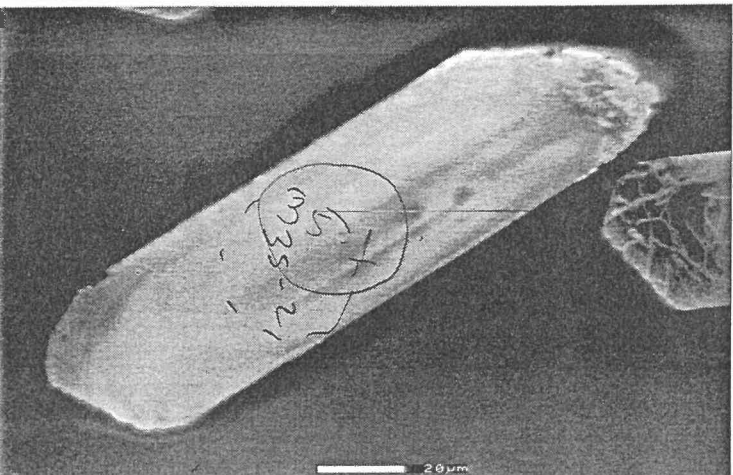


30kV ESD x735 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.98 20:25 P

9838A35S.TIF

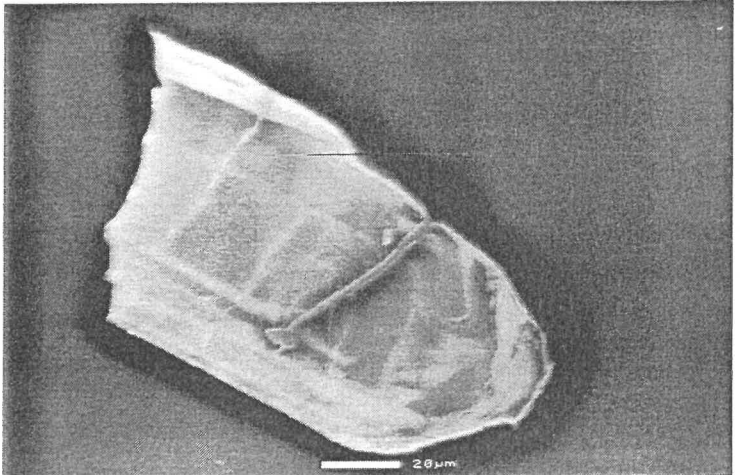


30kV ESD x685 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.98 20:28 P

9838A36S.TIF

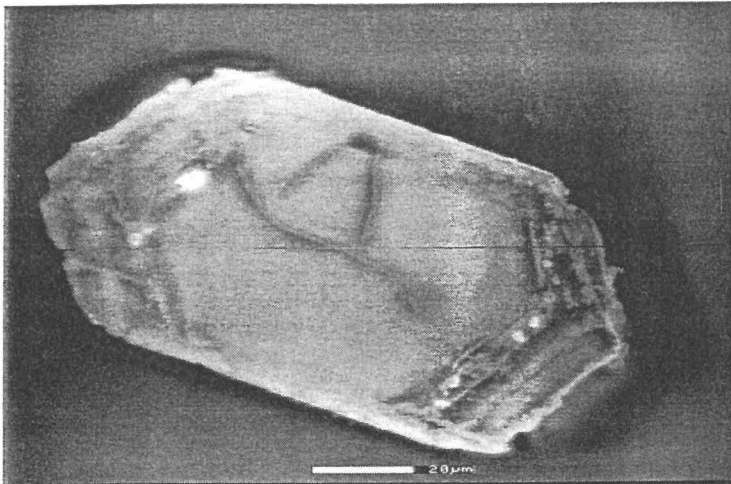


30kV ESD x865 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.08 20:31 P

9838A375.TIF

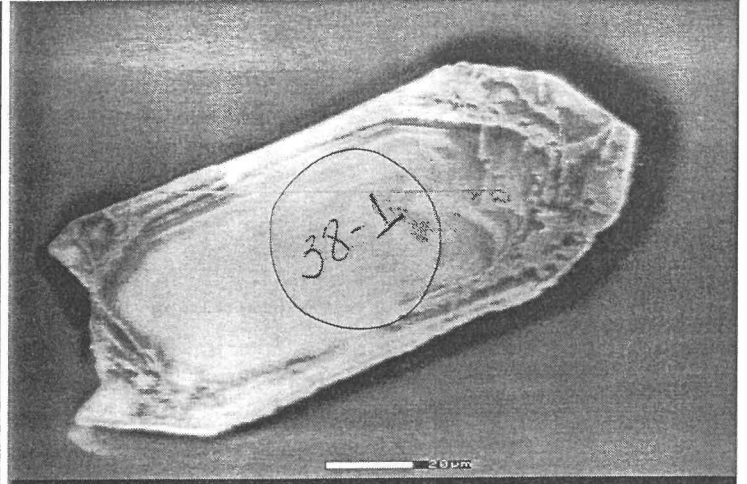


30kV ESD x755 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.08 20:33 P

9838A385.TIF

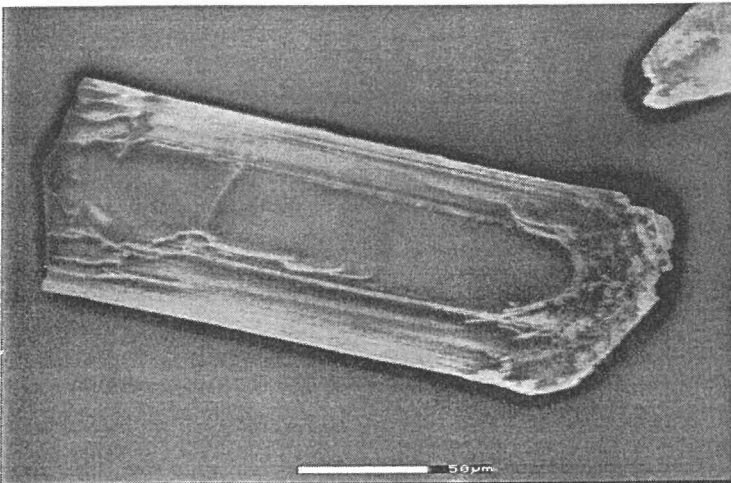

30kV ESD x445 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.08 20:35 P

9838A395.TIF

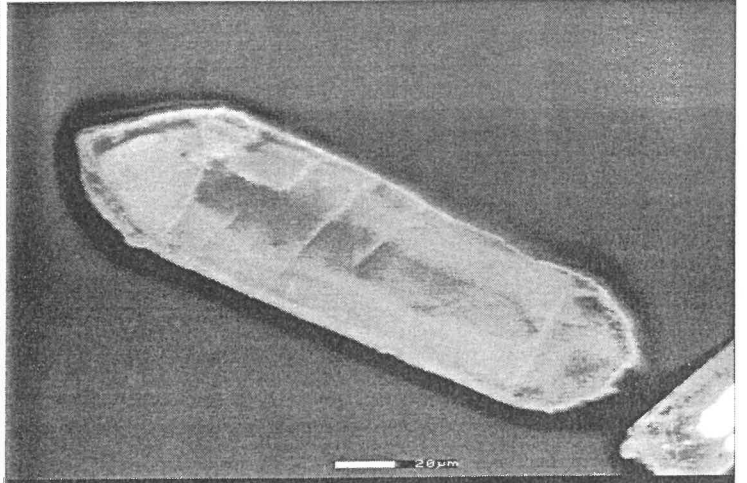

30kV ESD x525 D=9.7mm P=0.9T
Centre for Microscopy, UWA 98.09.08 20:38 P

9838A405.TIF