



30kV ESD x1100 D=9.4mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:16 P

9838b01s.tif

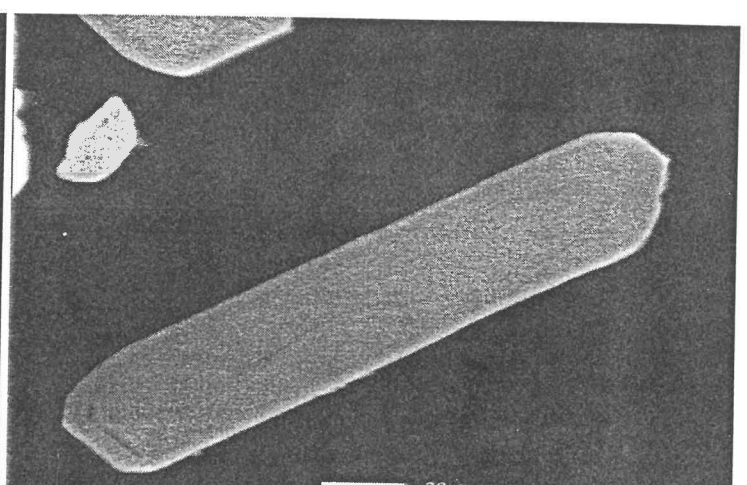


30kV ESD x710 D=9.4mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:20 P

9838b02s.tif

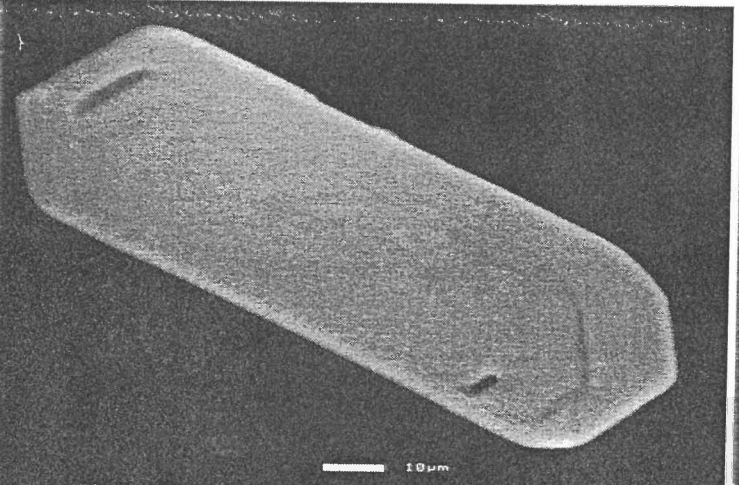


30kV ESD x1050 D=9.4mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:24 P

9838b03s.tif

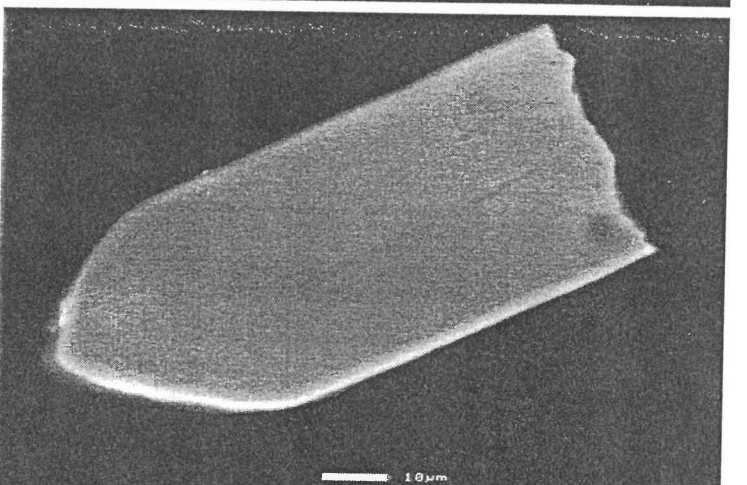


30kV ESD x1100 D=9.4mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:28 P

9838b04s.tif

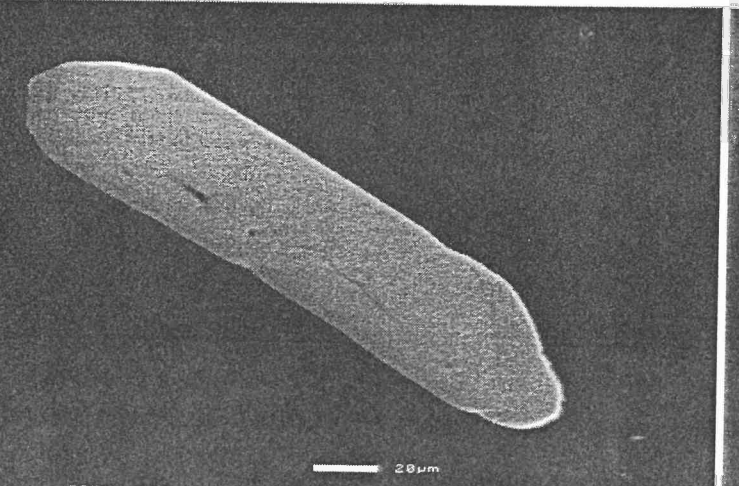


30kV ESD x545 D=9.4mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:31 P

9838b05s.tif

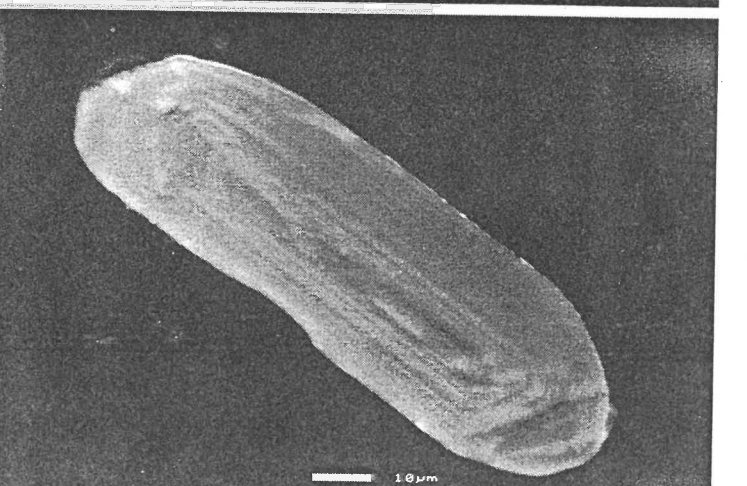


30kV ESD x1000 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:51 P

9838b06s.tif

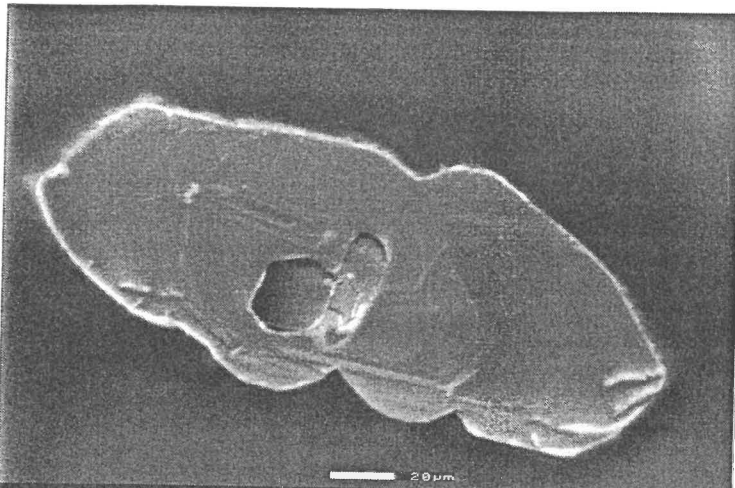


30kV ESD x555 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:55 P

9838b07s.tif

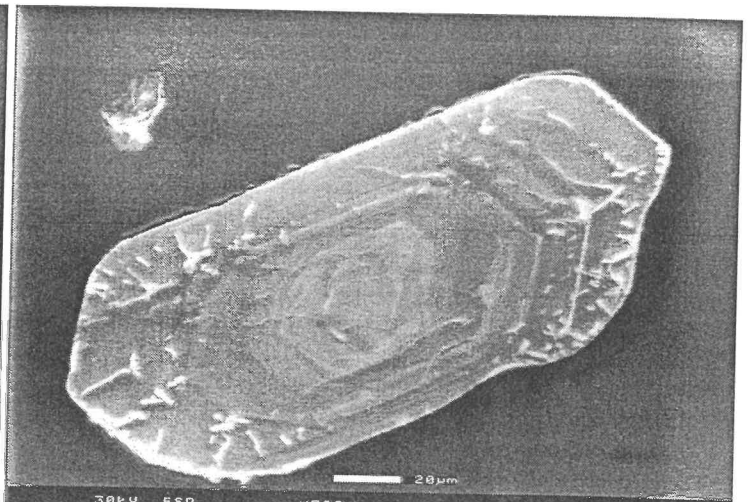


30kV ESD x580 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 17:59 P

9838b08s.tif

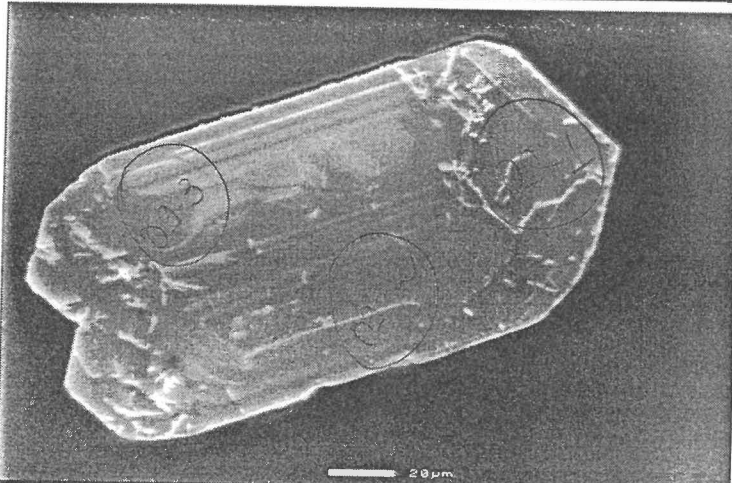


30kV ESD x575 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 18:02 P

9838b09s.tif

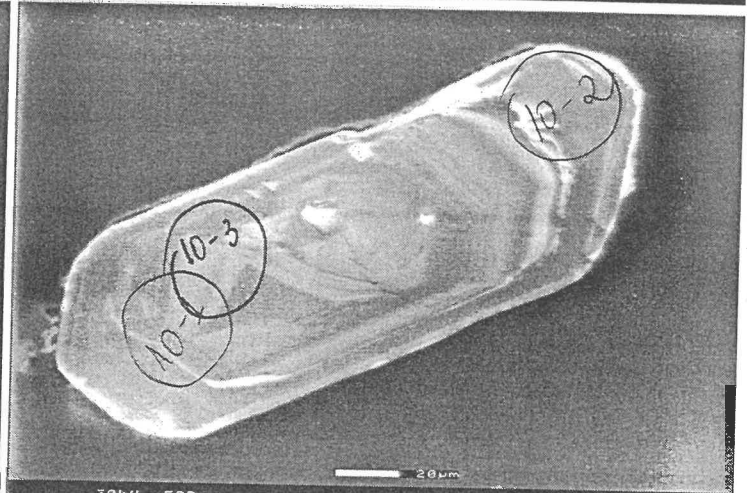


30kV ESD x555 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 18:06 P

9838b10s.tif

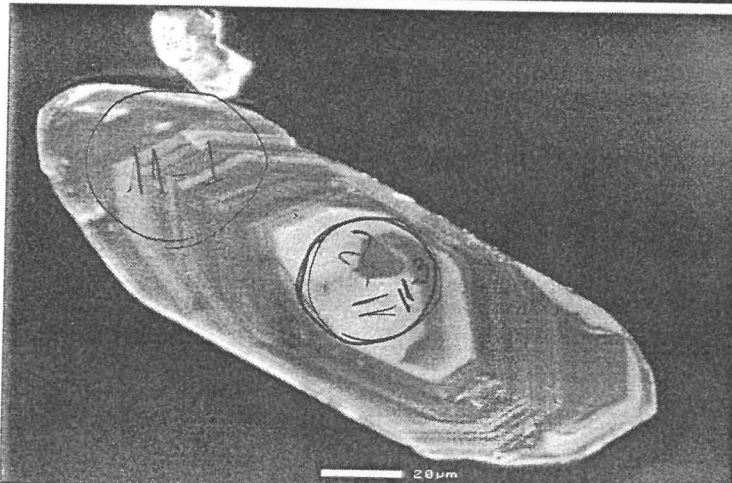

30kV ESD x705 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 18:08 P

9838b11s.tif






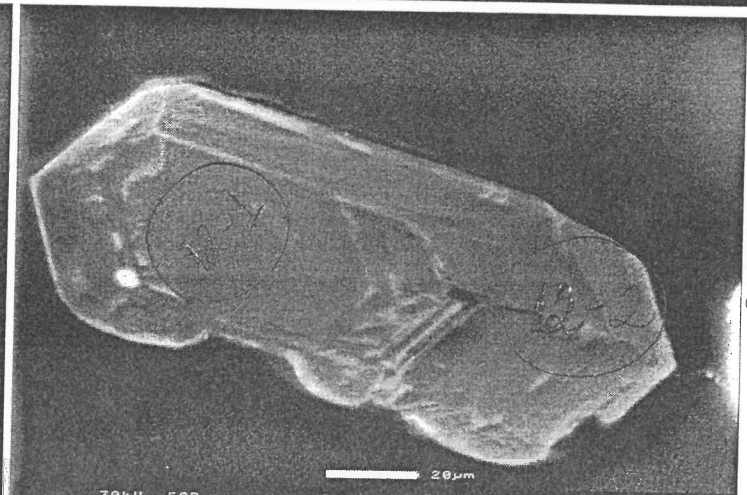








30kV ESD x780 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 18:14 P


9838b12s.tif

t/c


c/r
*

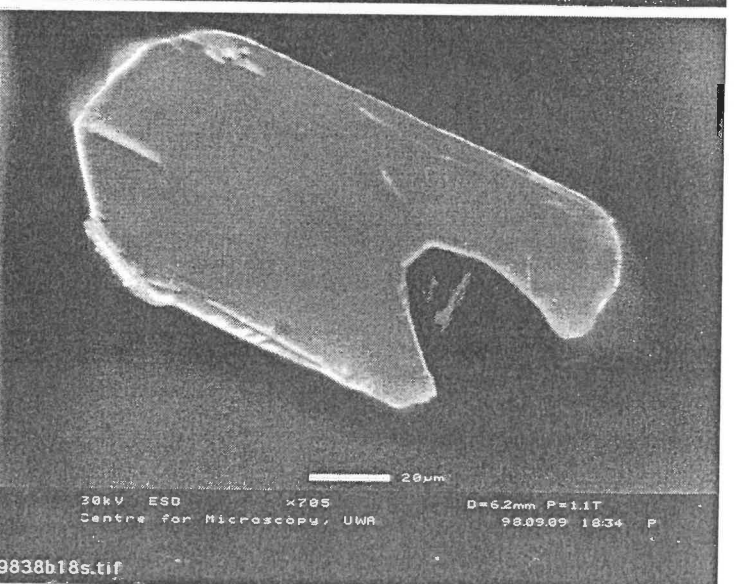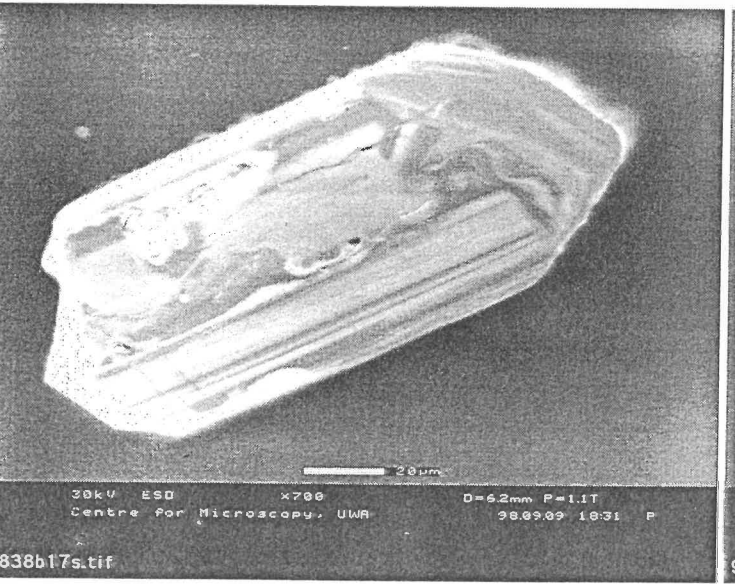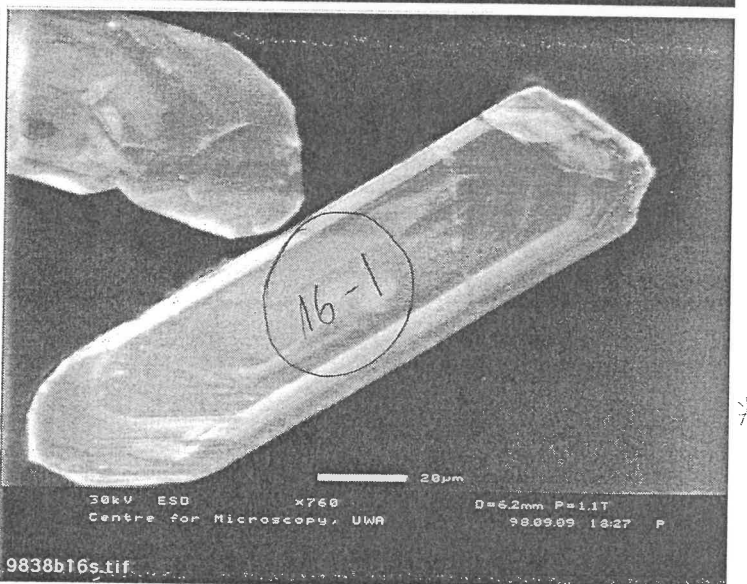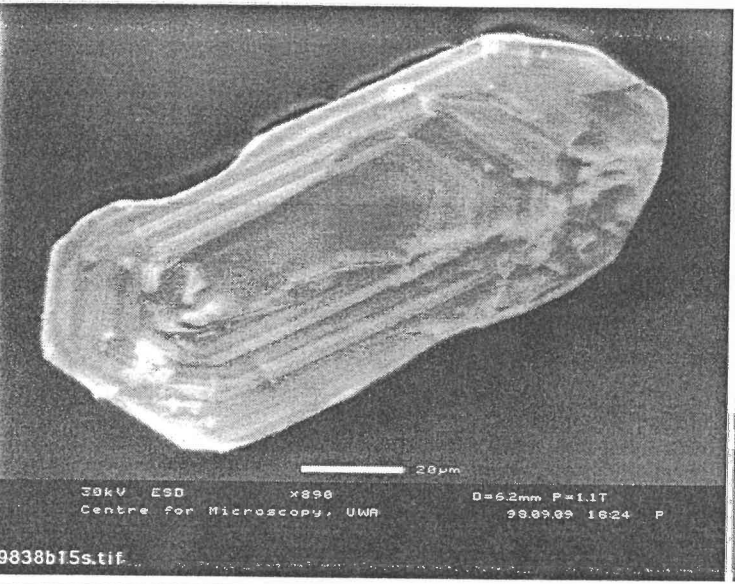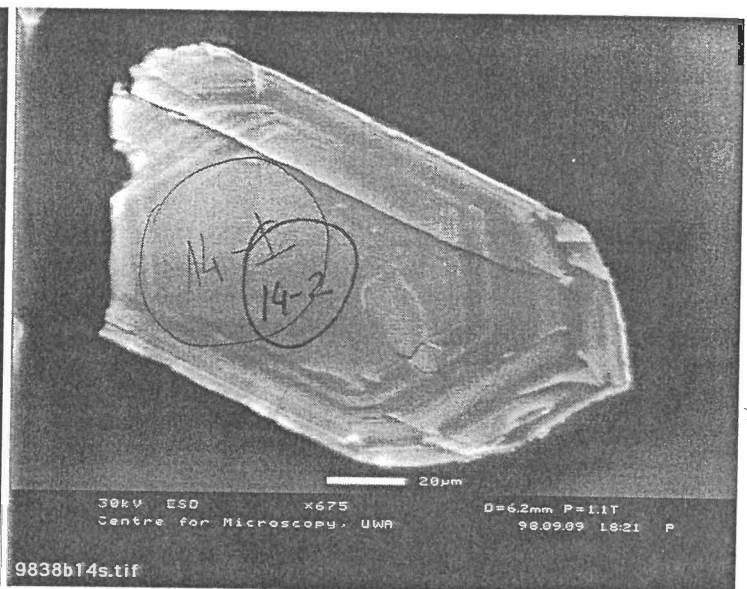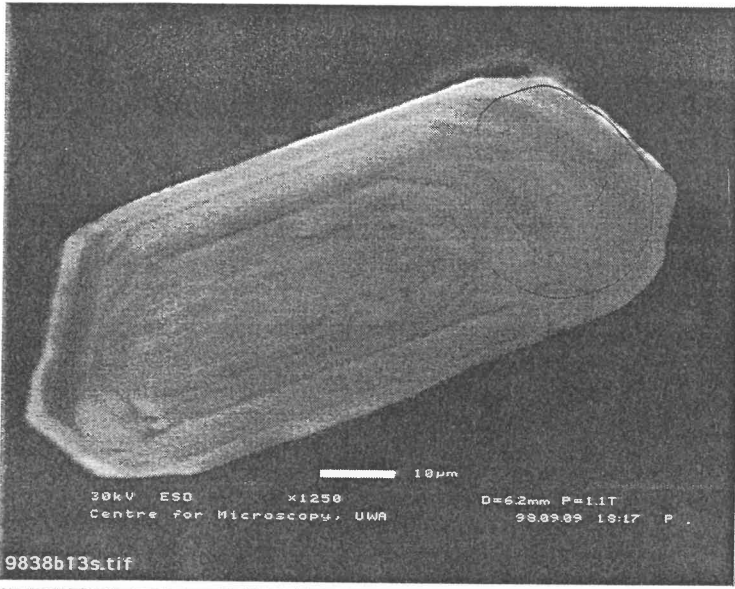

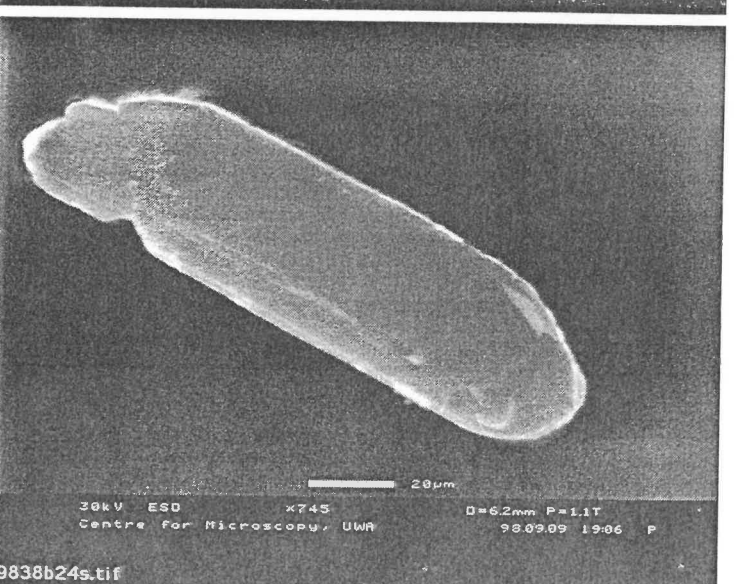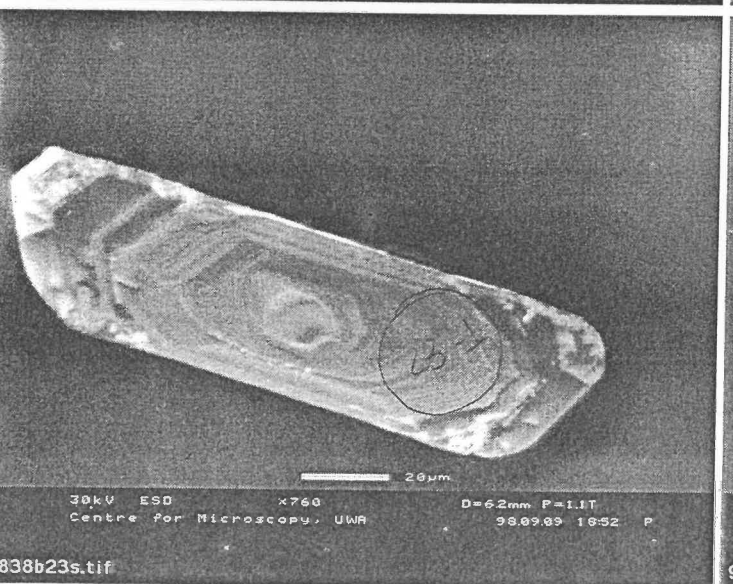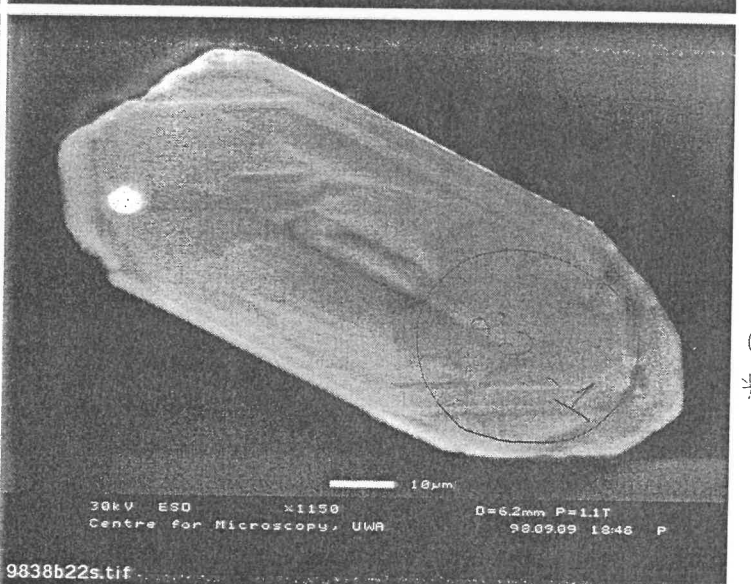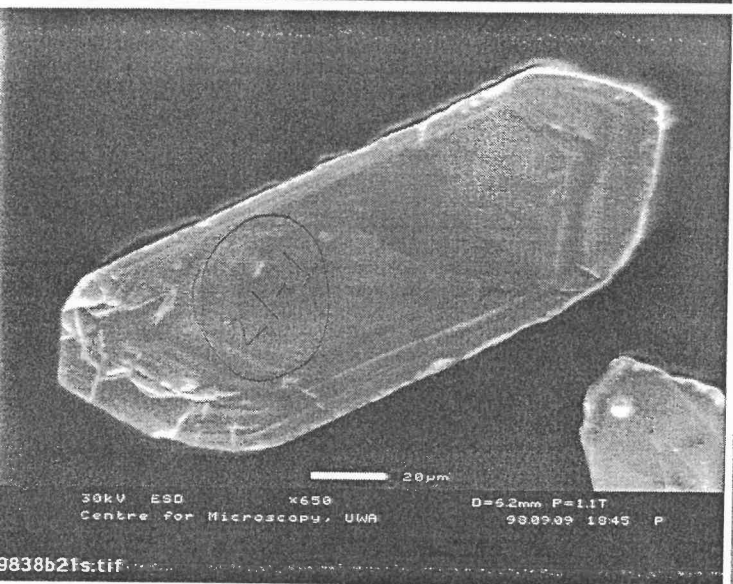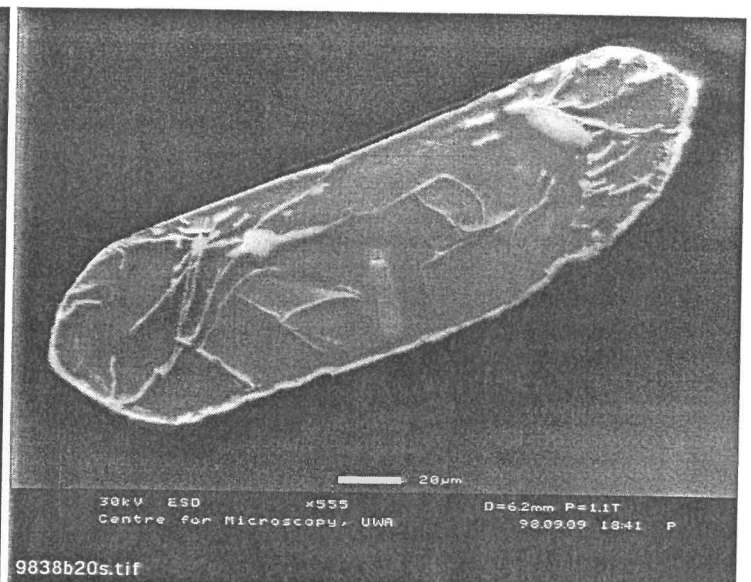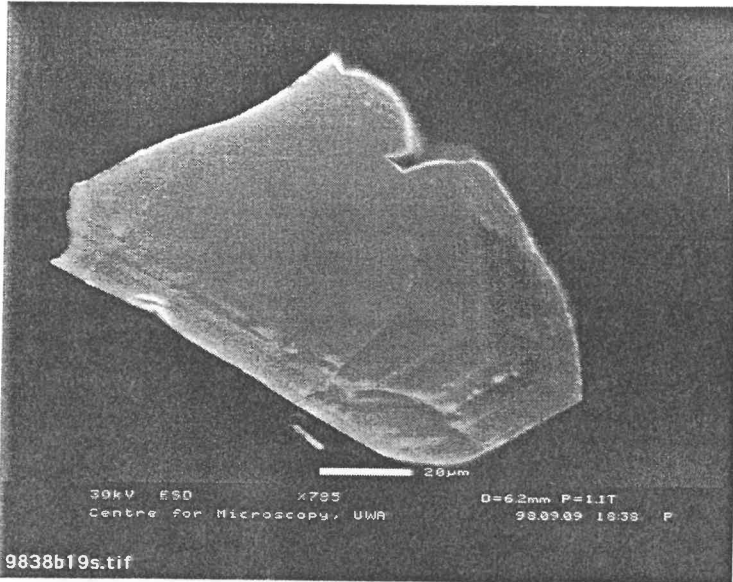


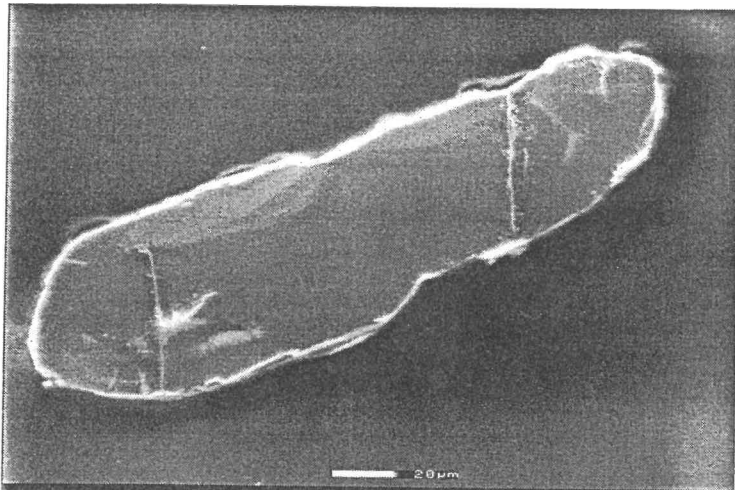


9838b25s.tif

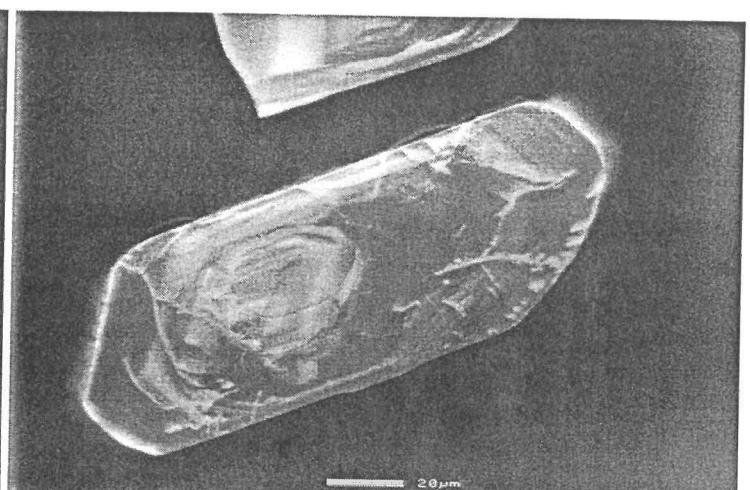


9838b26s.tif

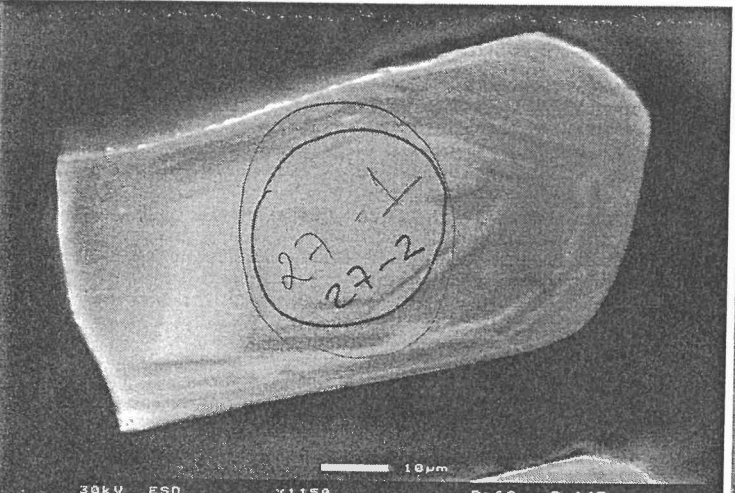


9838b27s.tif

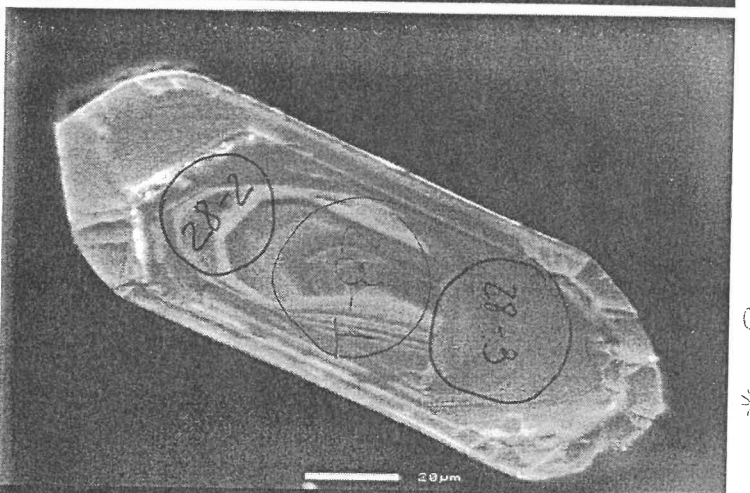

9838b28s.tif

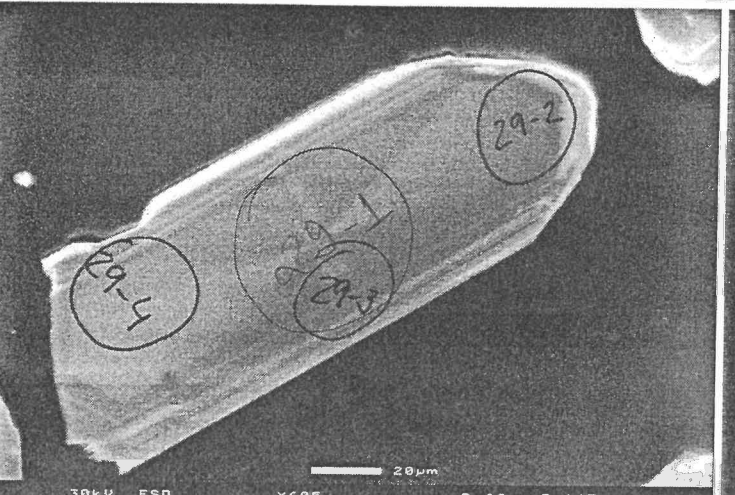


9838b29s.tif

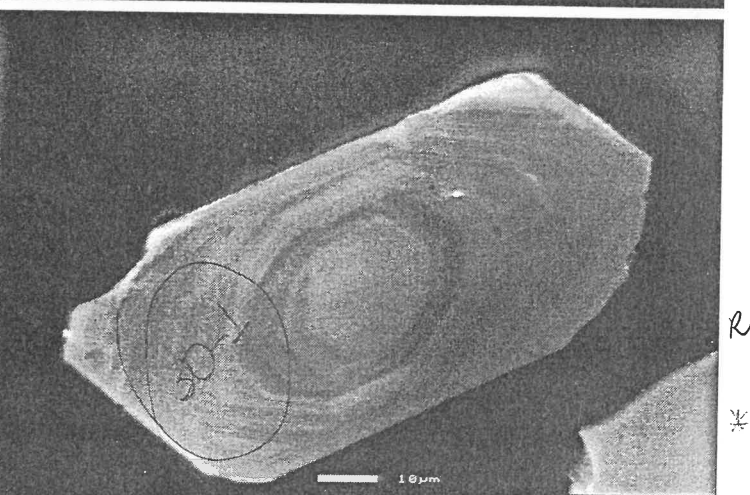

9838b30s.tif


C
*

R
*

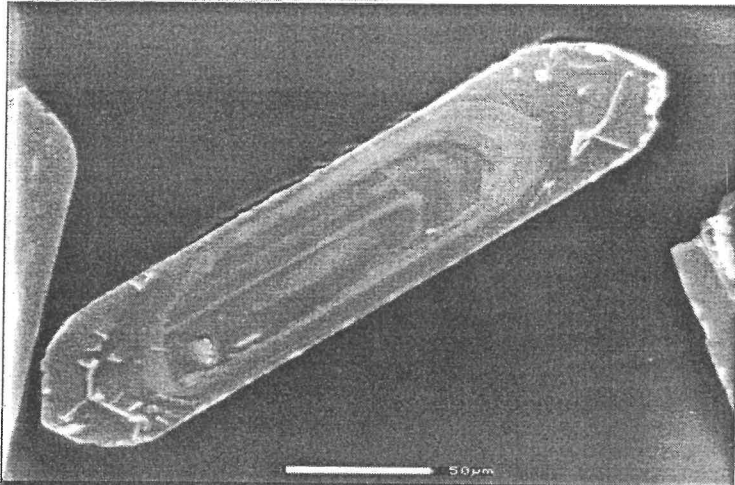


30kV ESD x495 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 19:28 P

9838b31s.tif

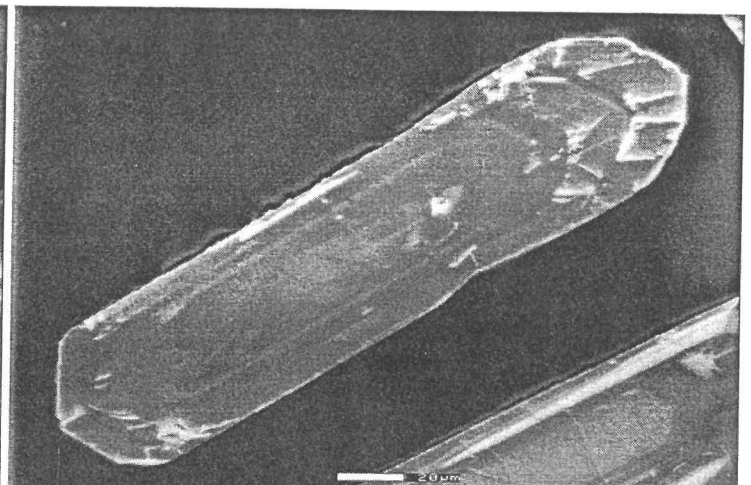


30kV ESD x575 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 19:32 P

9838b32s.tif

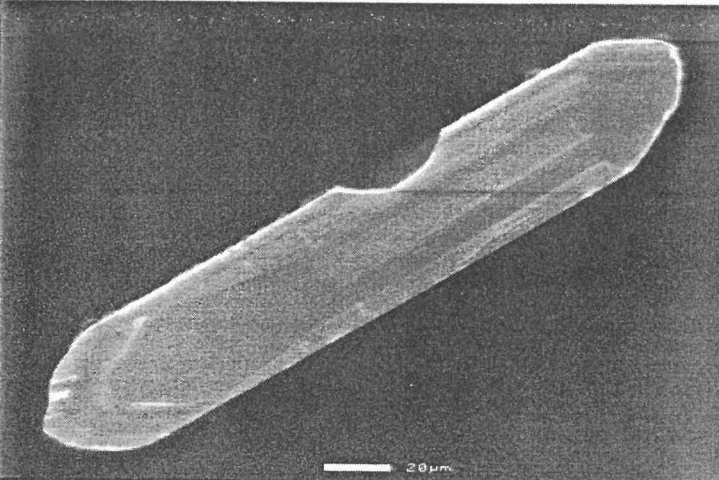


30kV ESD x568 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 19:34 P

9838b33s.tif

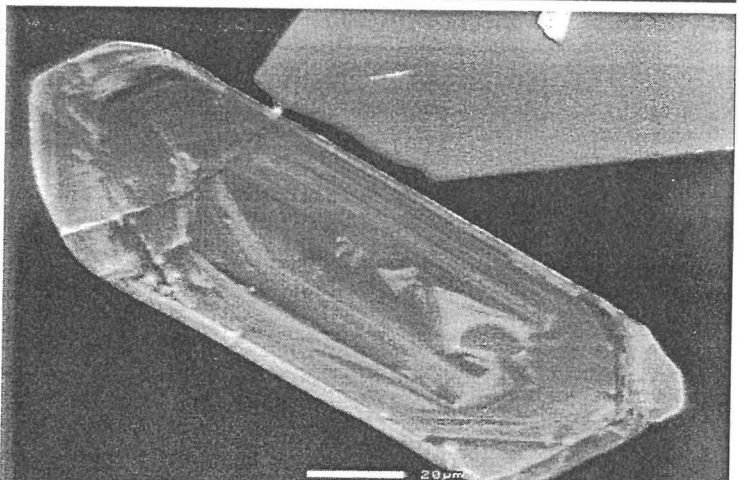


30kV ESD x855 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 19:37 P

9838b34s.tif

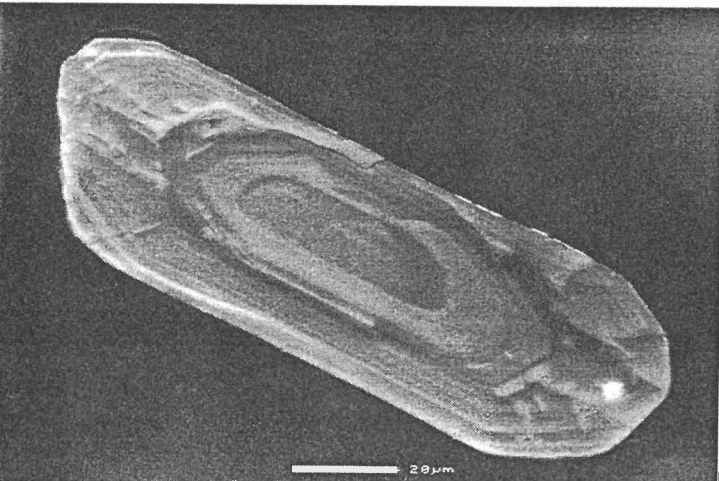

30kV ESD x908 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 19:40 P

9838b35s.tif

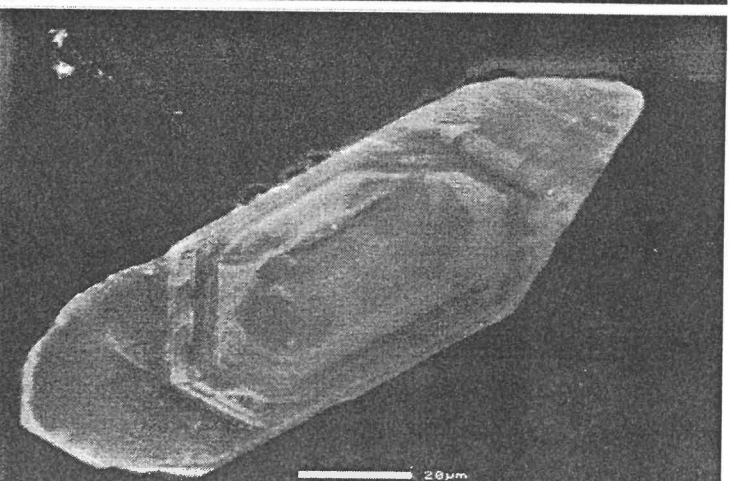

30kV ESD x985 D=6.2mm P=1.1T
Centre for Microscopy, UWA 98.09.09 19:42 P

9838b36s.tif

