


30kV ESD X420 D=9.9mm P=12T
Centre for Microscopy, UWA 98.11.10 2250 P

9876b05s.tif

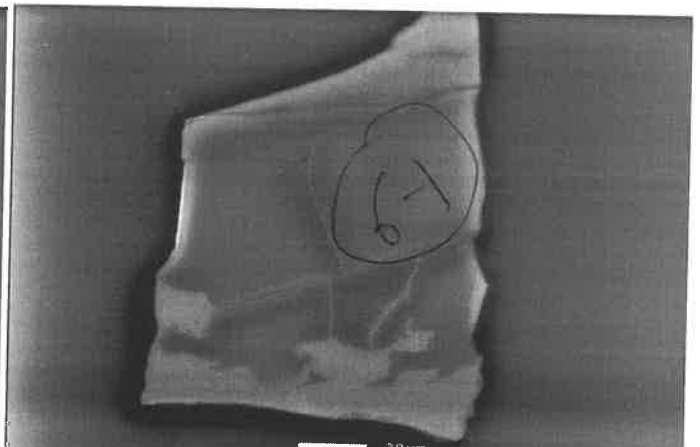


30kV ESD X630 D=9.9mm P=14T
Centre for Microscopy, UWA 98.11.10 2327 P

9876b06s.tif




30kV ESD X685 D=9.9mm P=13T
Centre for Microscopy, UWA 98.11.10 2330 P

9876b07s.tif

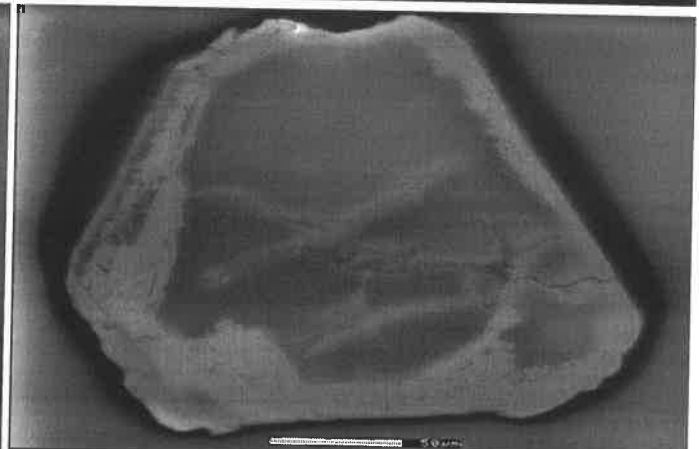


30kV ESD X490 D=9.9mm P=11T
Centre for Microscopy, UWA 98.11.10 2333 P

9876b08s.tif

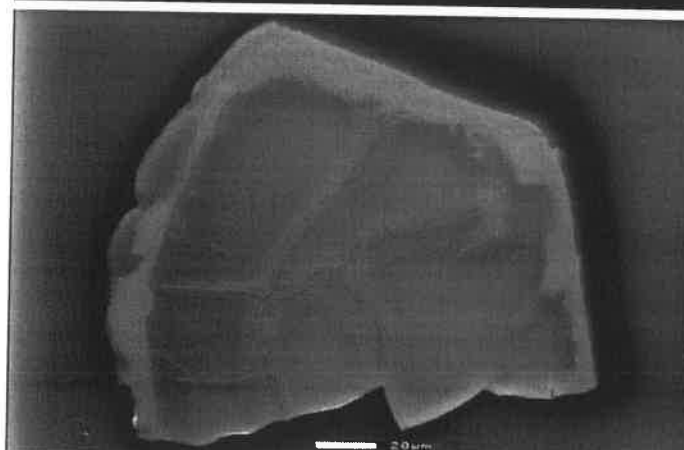


30kV ESD X560 D=9.9mm P=12T
Centre for Microscopy, UWA 98.11.10 2336 P

9876b09s.tif

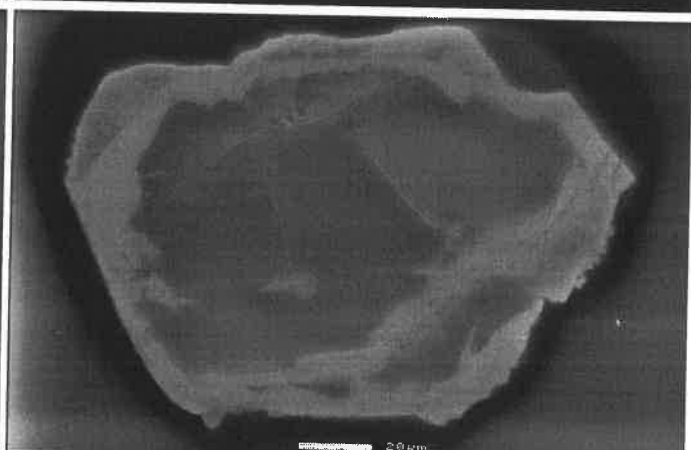


30kV ESD X670 D=9.9mm P=14T
Centre for Microscopy, UWA 98.11.10 2338 P

9876b10s.tif

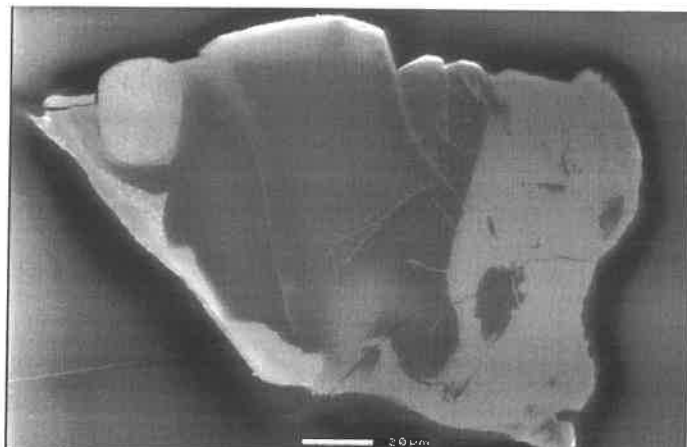


30kV ESD x655 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981110 2340 P

9876b11s.tif

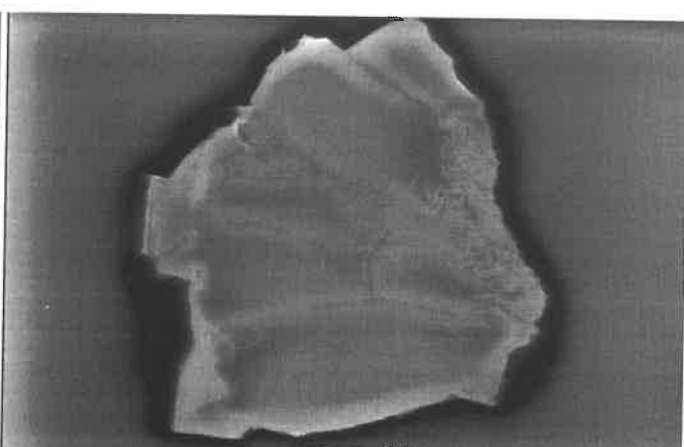


30kV ESD x510 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981110 2343 P

9876b12s.tif

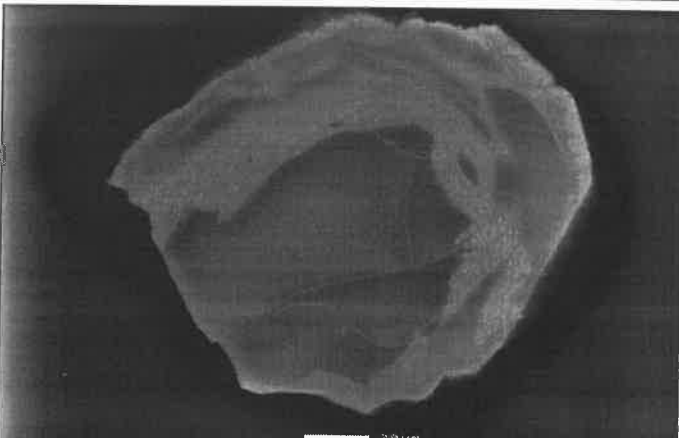


30kV ESD x600 D=9.9mm P=1.2T
Centre for Microscopy, UWA 981110 2346 P

9876b13s.tif

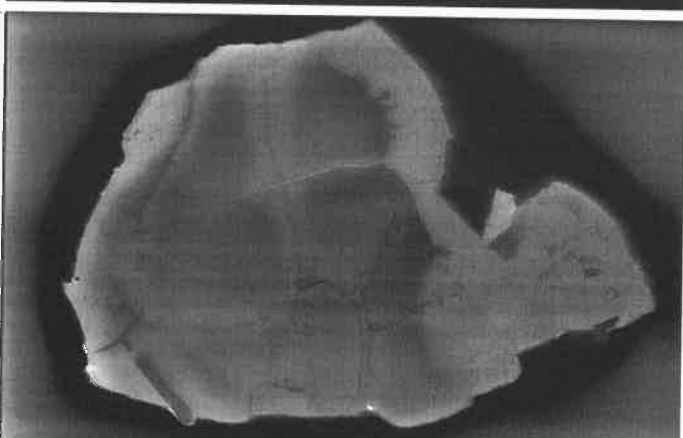


30kV ESD x700 D=9.9mm P=1.2T
Centre for Microscopy, UWA 981110 2350 P

9876b14s.tif

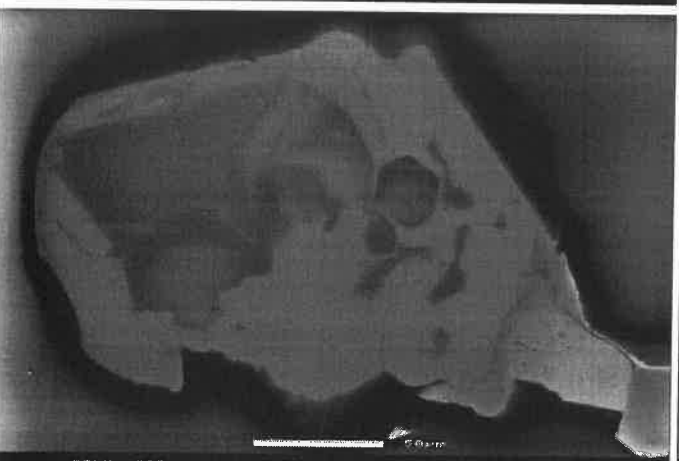


30kV ESD x485 D=9.9mm P=1.2T
Centre for Microscopy, UWA 981110 2354 P

9876b15s.tif

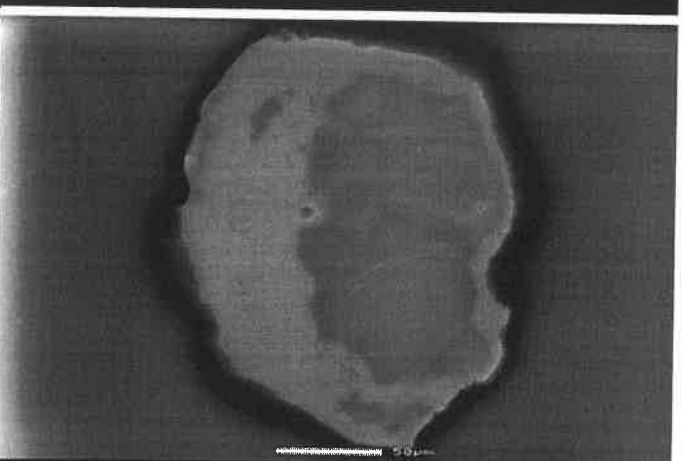


30kV ESD x400 D=9.9mm P=1.3T
Centre for Microscopy, UWA 981110 2357 P

9876b16s.tif

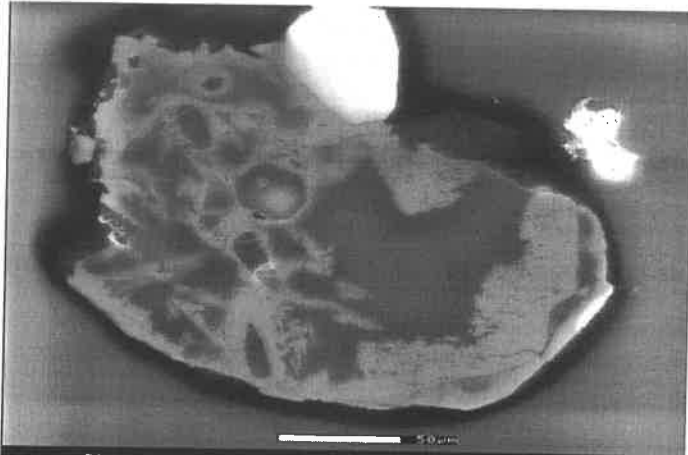


20kV ESD x450 D=9.9mm P=10T
Centre for Microscopy, UWA 98.11.11 0001 P

9876b17s.tif

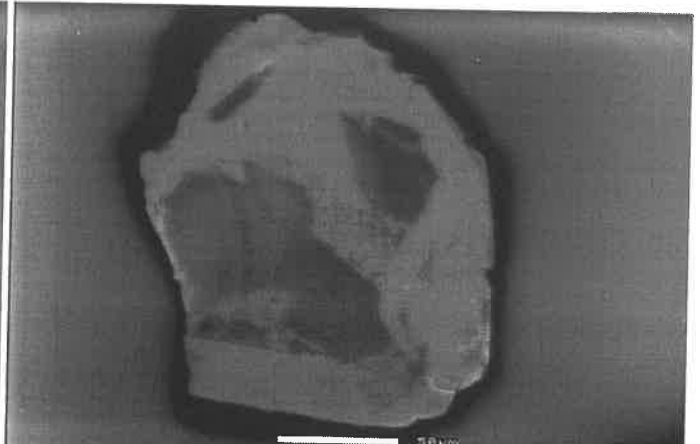


20kV ESD x450 D=9.9mm P=10T
Centre for Microscopy, UWA 98.11.11 0004 P

9876b18s.tif

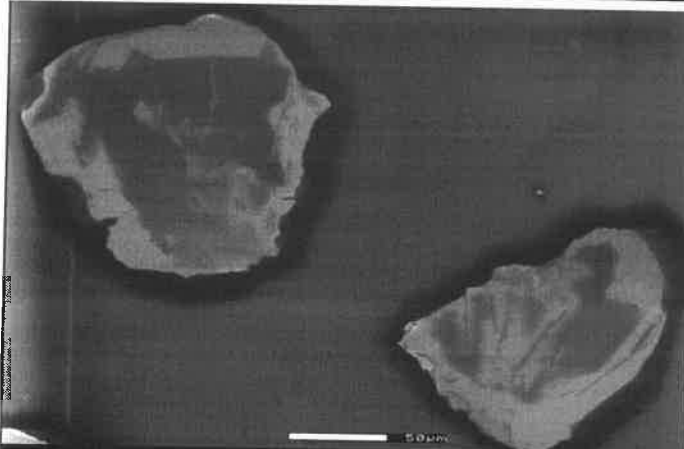


20kV ESD x370 D=9.9mm P=10T
Centre for Microscopy, UWA 98.11.11 0005 P

9876b19s.tif

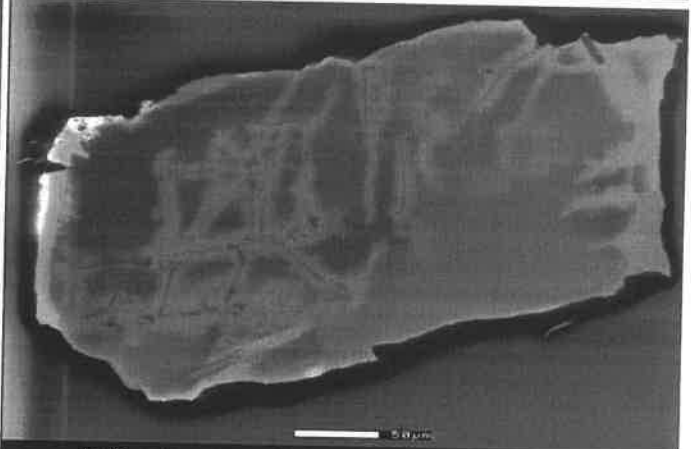


20kV ESD x315 D=9.9mm P=10T
Centre for Microscopy, UWA 98.11.11 0009 P

9876b20s.tif

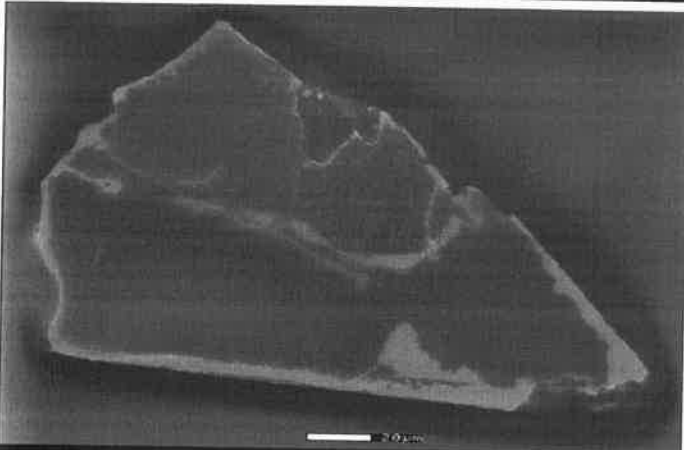


20kV ESD x600 D=9.9mm P=13T
Centre for Microscopy, UWA 98.11.11 0012 P

9876b21s.tif

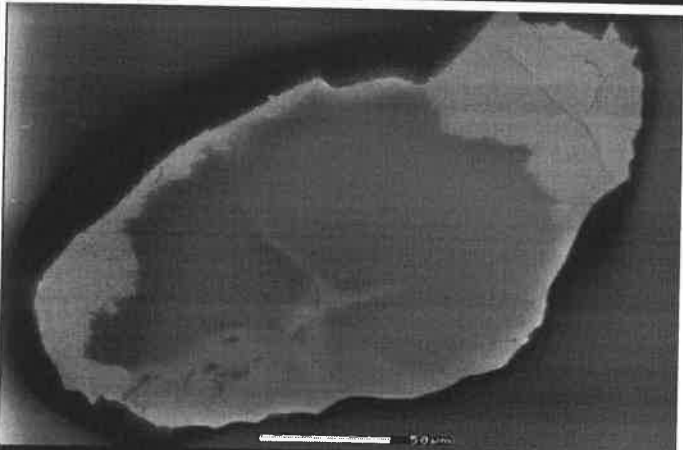


20kV ESD x490 D=9.9mm P=14T
Centre for Microscopy, UWA 98.11.11 0014 P

9876b22s.tif

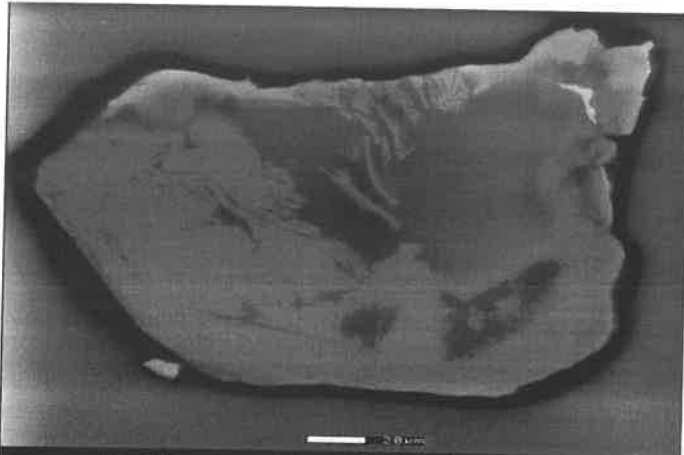


30kV ESD X450 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981111 0816 P

9876b23s.tif

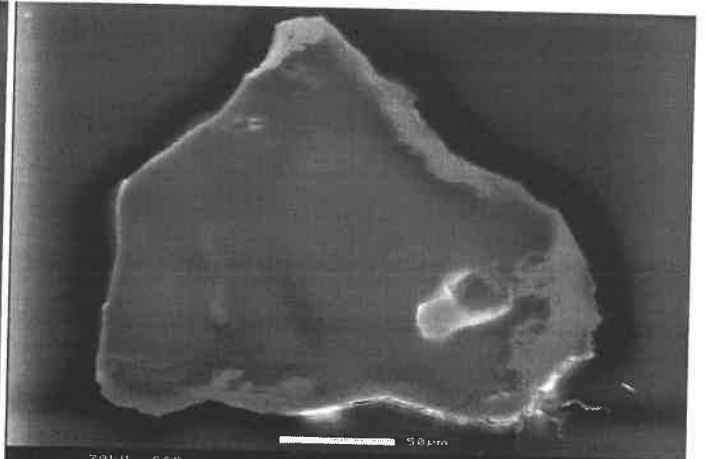


30kV ESD X435 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981111 0819 P

9876b24s.tif

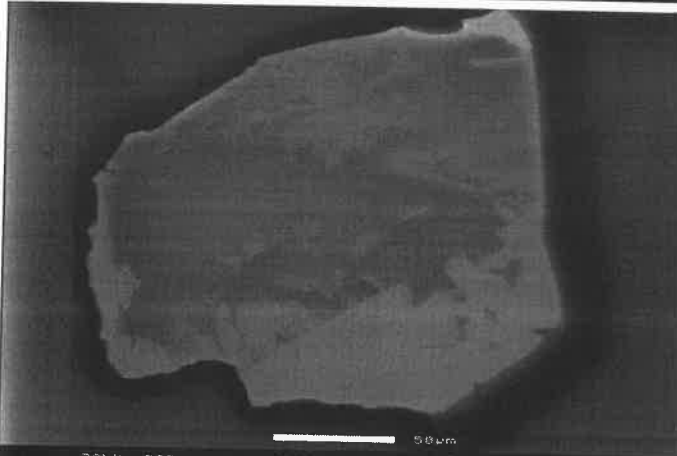


30kV ESD X450 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981111 0822 P

9876b25s.tif

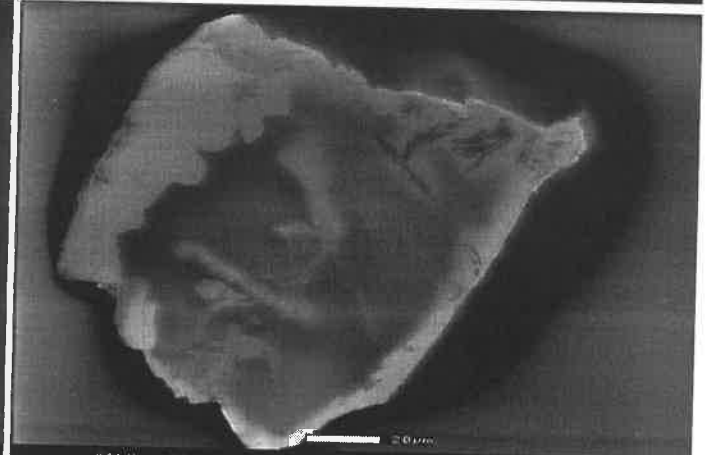


30kV ESD X685 D=10mm P=1.1T
Centre for Microscopy, UWA 981111 0825 P

9876b26s.tif

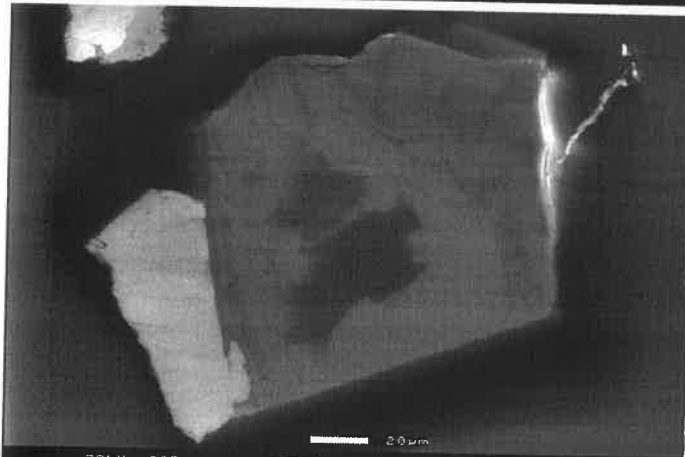

30kV ESD X635 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981111 0828 P

9876b27s.tif

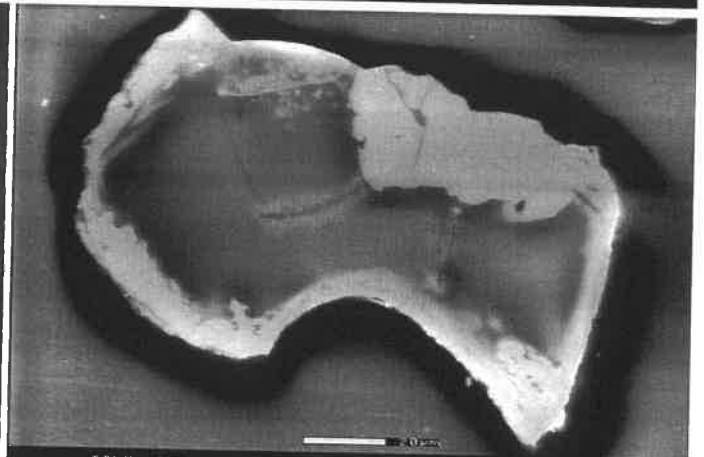

30kV ESD X770 D=9.9mm P=1.1T
Centre for Microscopy, UWA 981111 0832 P

9876b28s.tif

UWA 98-76, B: 97969082A (6) 11.11.98

