



30kV ESD X830 D=10mm P=11T  
Centre for Microscopy, UWA 98.11.14 2346 P

9876d12s.tif

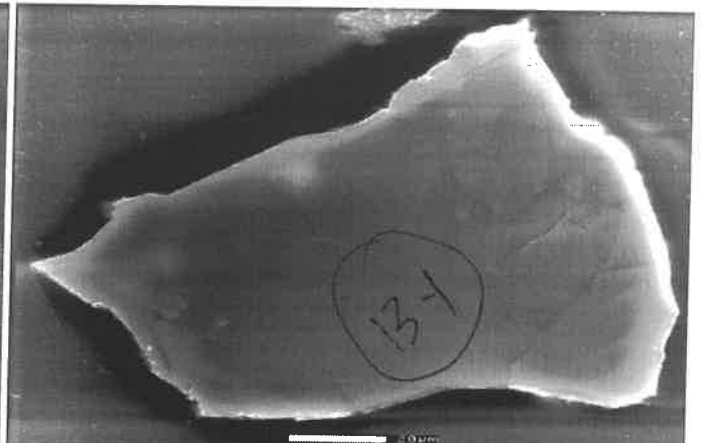


30kV ESD X905 D=10mm P=15T  
Centre for Microscopy, UWA 98.11.14 2348 P

9876d13s.tif

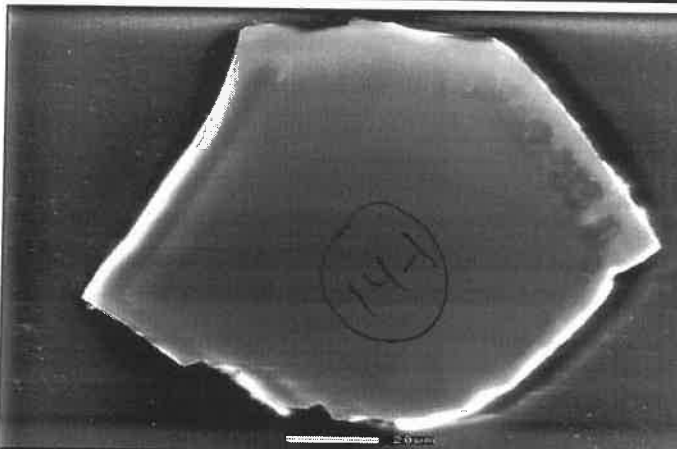


30kV ESD X865 D=10mm P=13T  
Centre for Microscopy, UWA 98.11.14 2351 P

9876d14s.tif

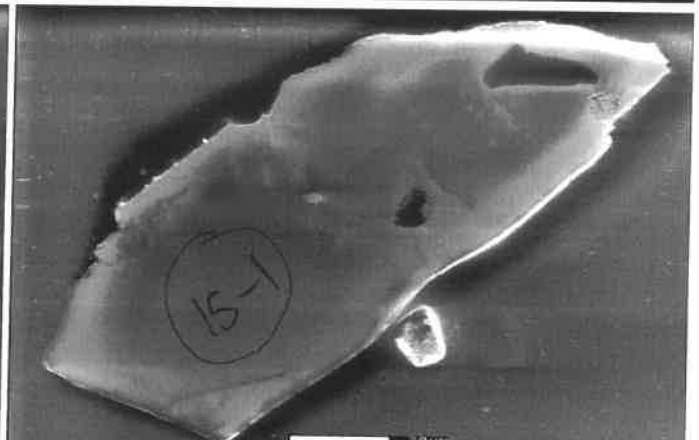


30kV ESD X920 D=10mm P=12T  
Centre for Microscopy, UWA 98.11.14 2352 P

9876d15s.tif

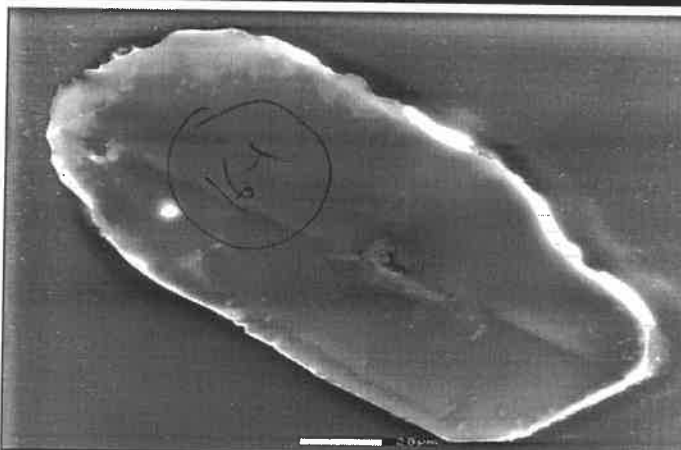


30kV ESD X755 D=10mm P=13T  
Centre for Microscopy, UWA 98.11.14 2354 P

9876d16s.tif

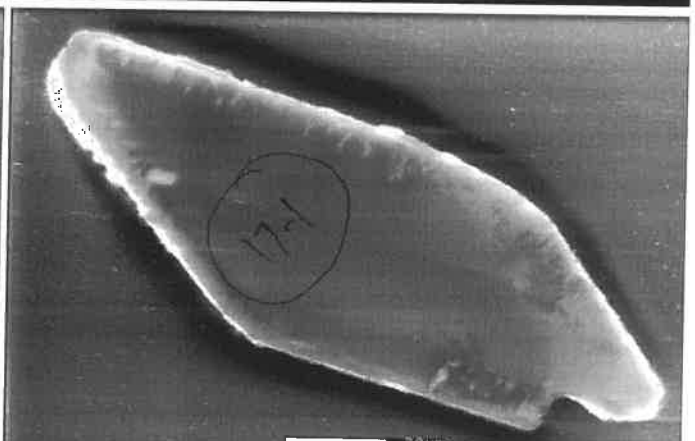


30kV ESD X940 D=10mm P=12T  
Centre for Microscopy, UWA 98.11.14 2355 P

9876d17s.tif

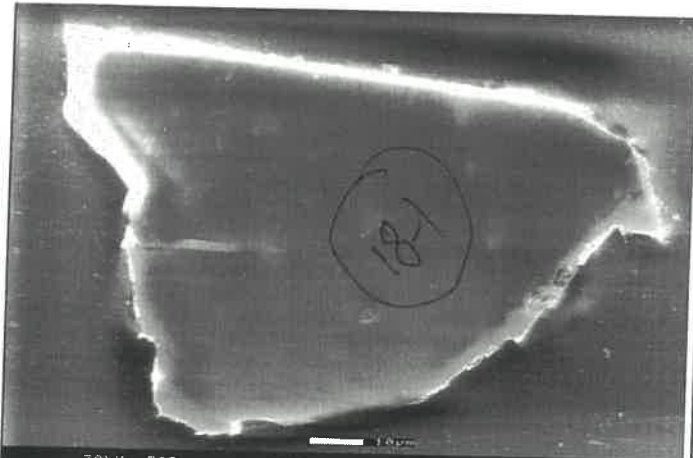


30kV ESD x1000 D=10mm P=1.37  
Centre for Microscopy, UWA 98.11.15 0058 P

9876d18s.tif

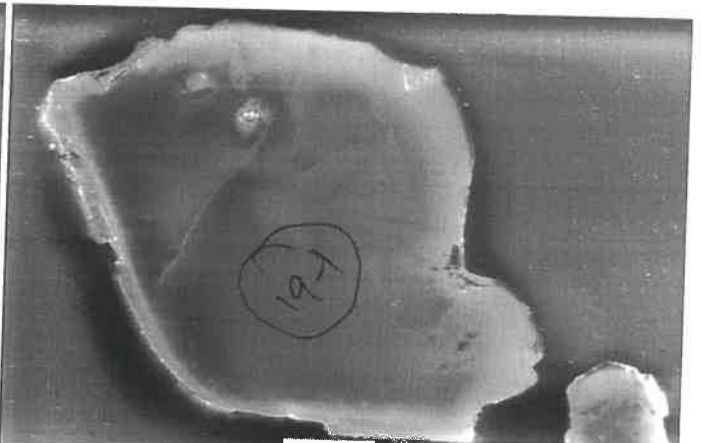


30kV ESD x665 D=10mm P=1.17  
Centre for Microscopy, UWA 98.11.15 0061 P

9876d19s.tif

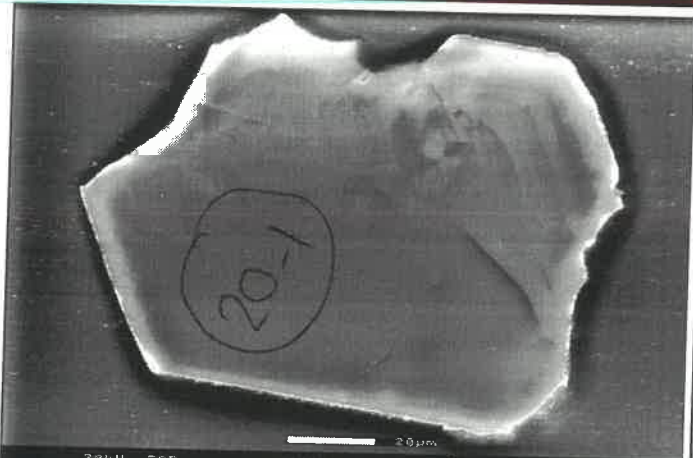


30kV ESD x815 D=10mm P=1.17  
Centre for Microscopy, UWA 98.11.15 0063 P

9876d20s.tif

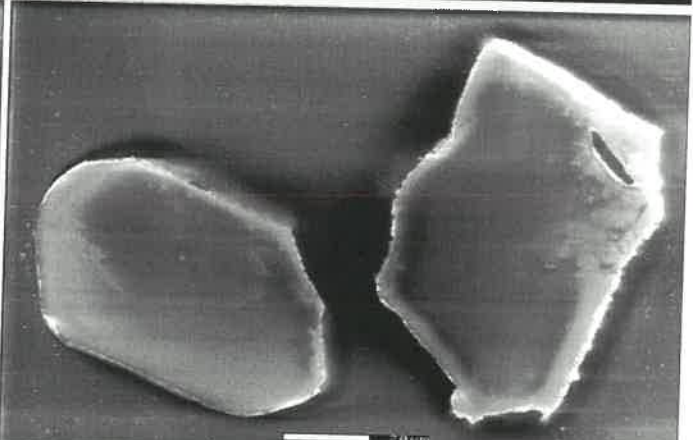


30kV ESD x815 D=10mm P=1.17  
Centre for Microscopy, UWA 98.11.15 0064 P

9876d21s.tif

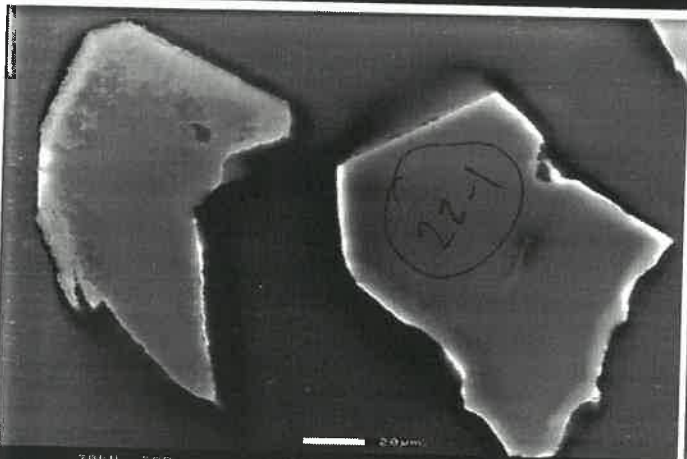


30kV ESD x565 D=10mm P=1.47  
Centre for Microscopy, UWA 98.11.15 0066 P

9876d22s.tif

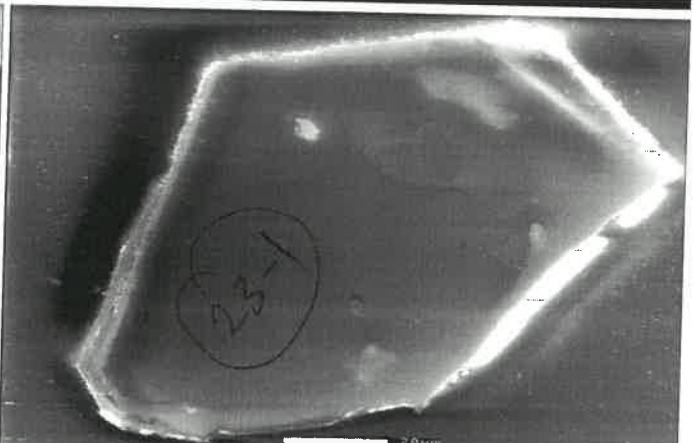


30kV ESD x590 D=10mm P=1.47  
Centre for Microscopy, UWA 98.11.15 0068 P

9876d23s.tif

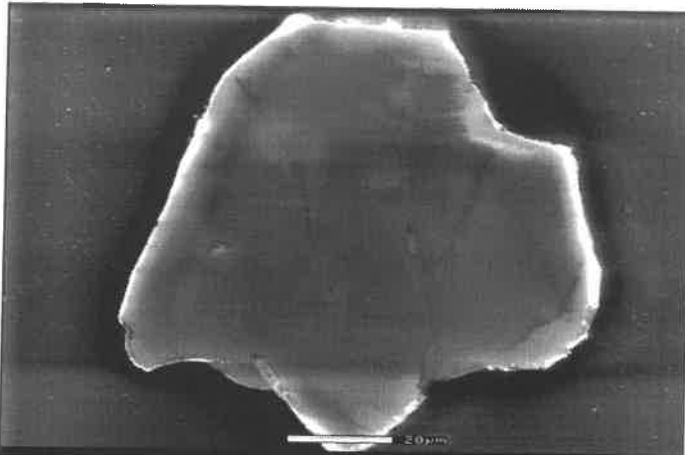


20kV ESD X990 D=10mm F=1.5T  
Centre for Microscopy, UWA 201115 00:10 P

9876d24s.tif

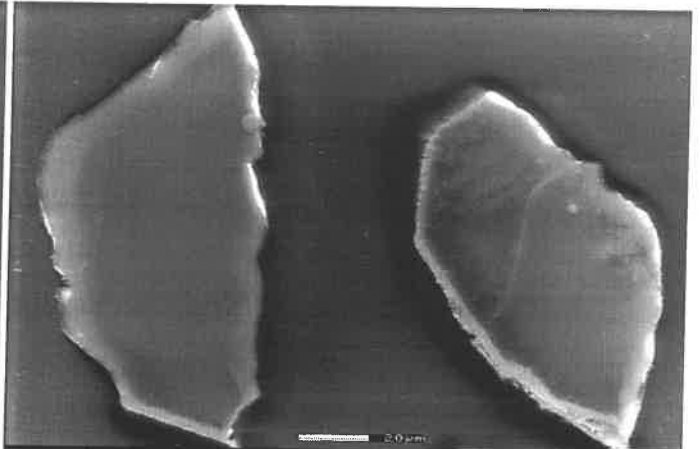

20kV ESD X670 D=10mm F=1.5T  
Centre for Microscopy, UWA 201115 00:12 P

9876d25s.tif

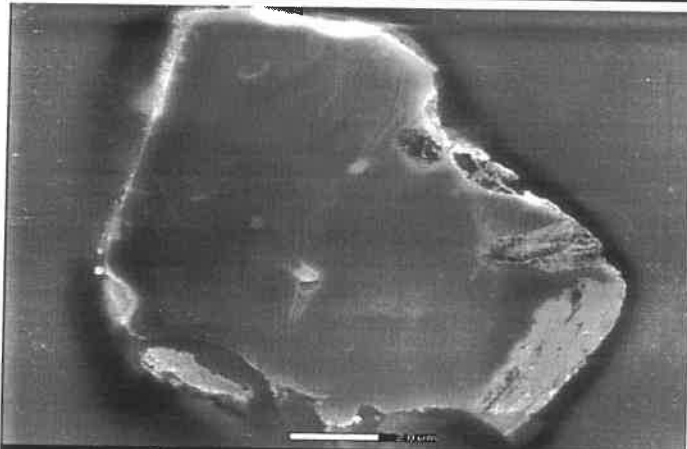

20kV ESD X845 D=10mm F=1.5T  
Centre for Microscopy, UWA 201115 00:13 P

9876d26s.tif