



30kV ESD X1200 D=9.7mm P=1.2T  
Centre for Microscopy, UWA 98.12.04 12:46 P

9884d10s.tif

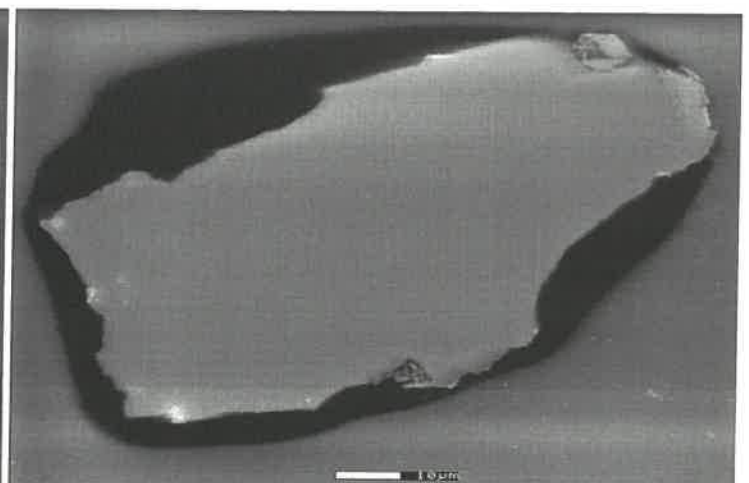


30kV ESD X1100 D=9.7mm P=1.2T  
Centre for Microscopy, UWA 98.12.04 12:49 P

9884d11s.tif

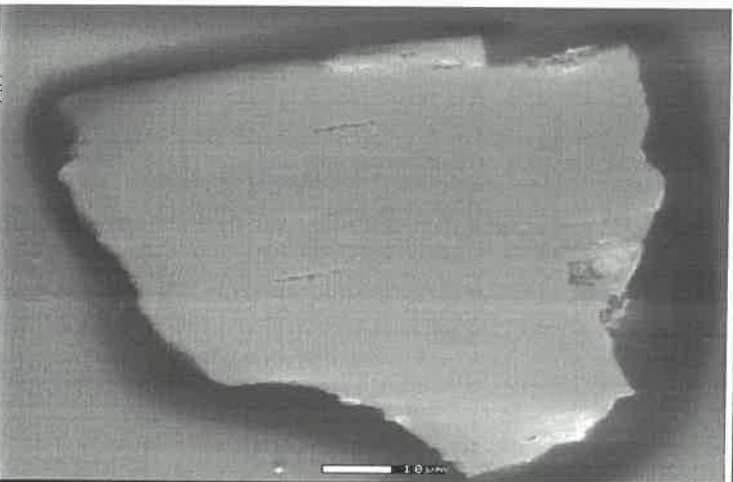


30kV ESD X1200 D=9.7mm P=1.2T  
Centre for Microscopy, UWA 98.12.04 12:52 P

9884d12s.tif

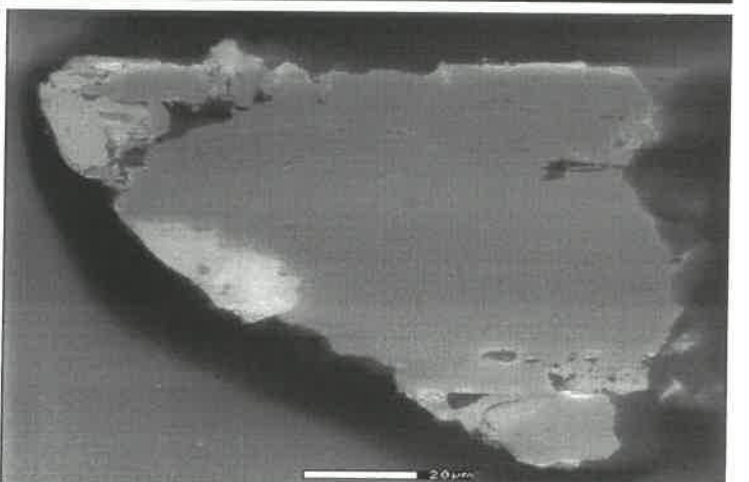


30kV ESD X990 D=9.7mm P=1.2T  
Centre for Microscopy, UWA 98.12.04 12:55 P

9884d13s.tif

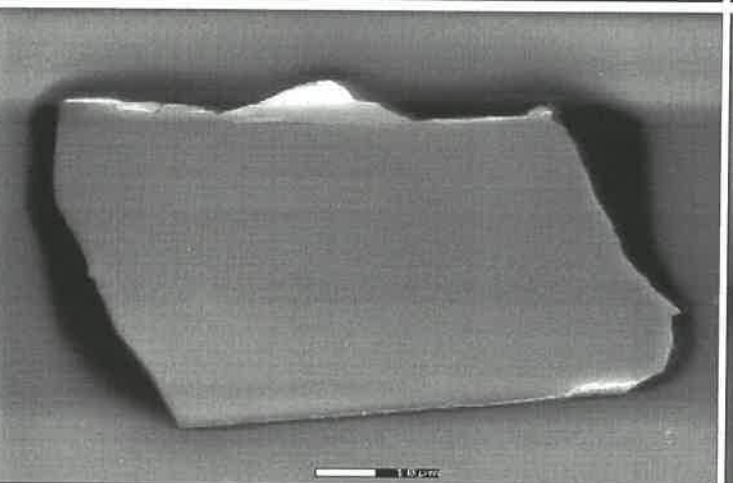

30kV ESD X1050 D=9.7mm P=1.2T  
Centre for Microscopy, UWA 98.12.04 13:00 P

9884d14s.tif

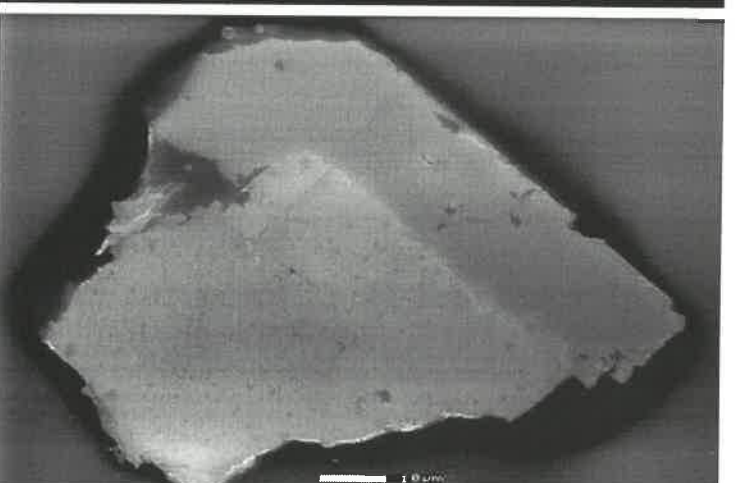

30kV ESD X1150 D=9.7mm P=1.2T  
Centre for Microscopy, UWA 98.12.04 13:03 P

9884d15s.tif