



30kV ESD X870 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 10:32 P

9889a15s.tif

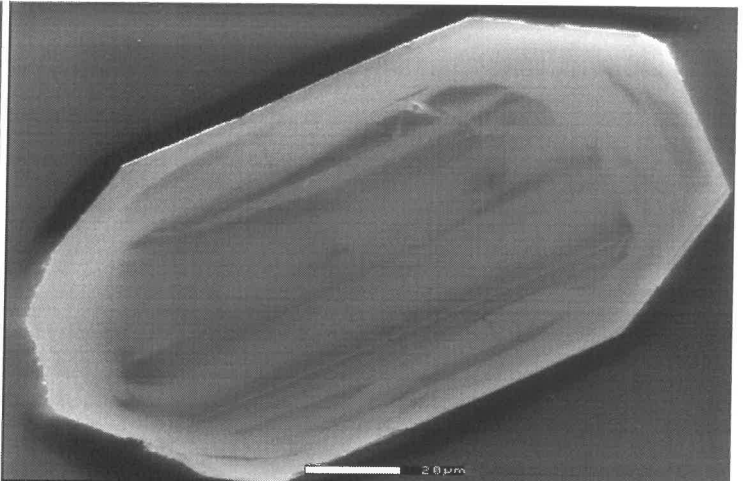


30kV ESD X825 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 10:34 P

9889a16s.tif

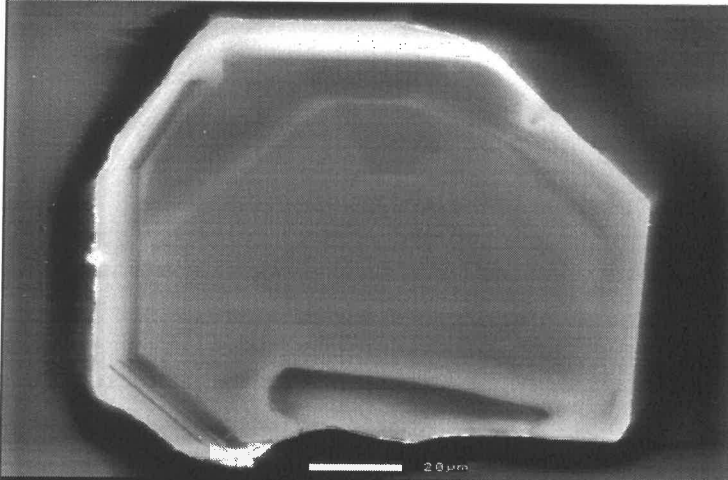


30kV ESD X815 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 11:43 P

9889a17s.tif

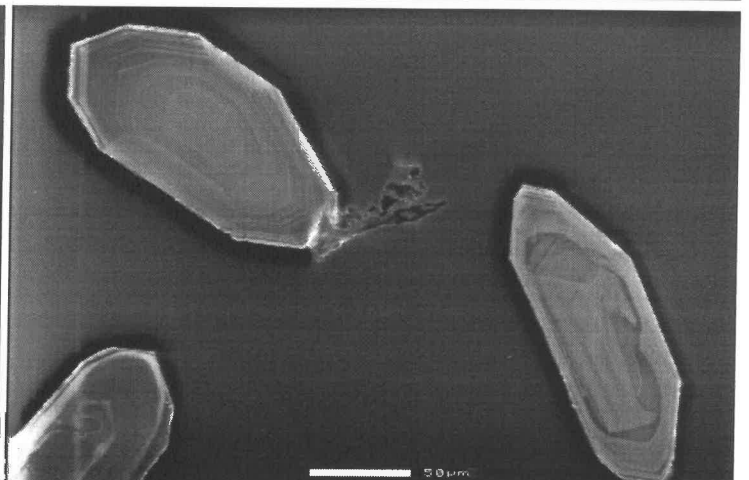


30kV ESD X335 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 11:46 P

9889a18s.tif

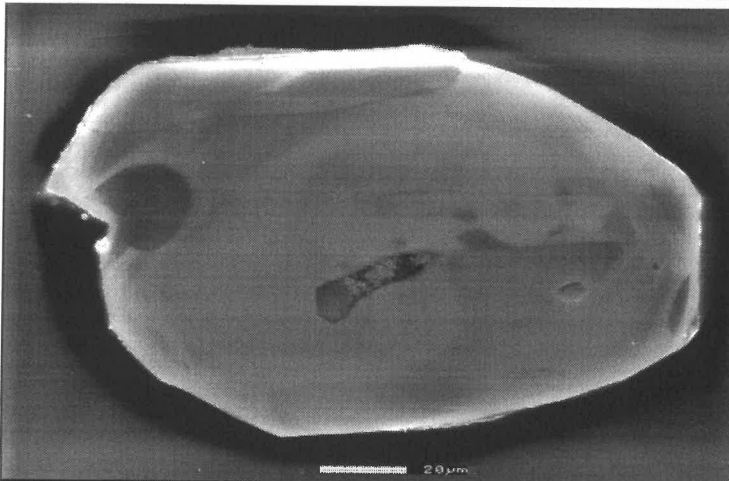


30kV ESD X750 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 11:47 P

9889a19s.tif

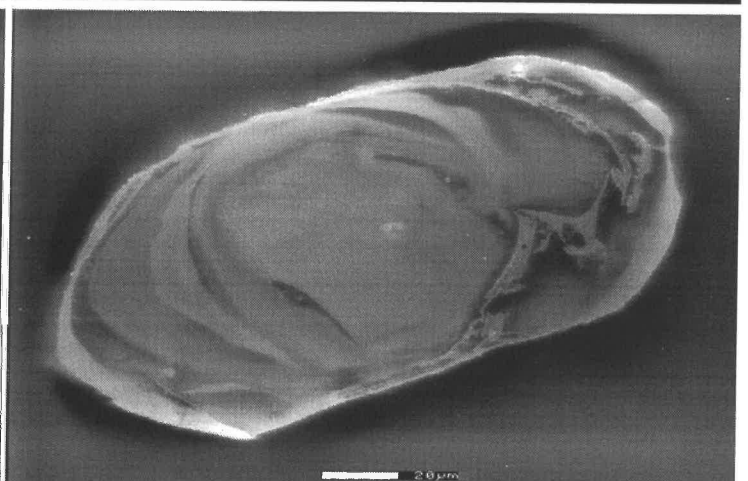


30kV ESD X670 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 11:50 P

9889a20s.tif

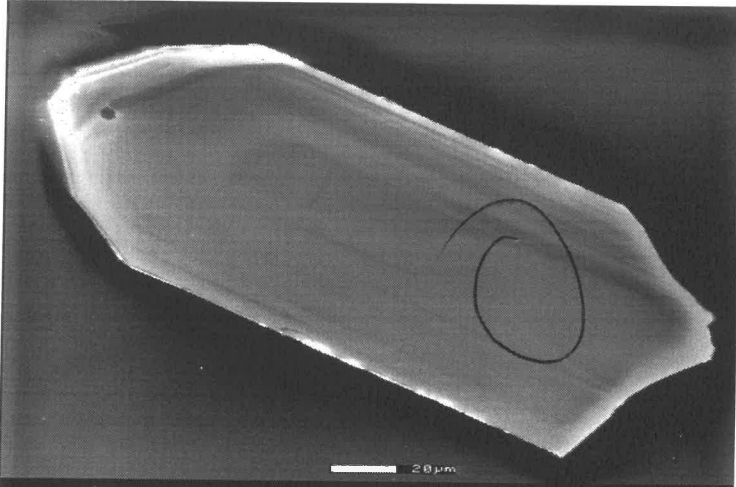


30kV ESD X560 D=10mm P=0.9T
Centre for Microscopy, UWA 981206 11:52 P

9889a21s.tif

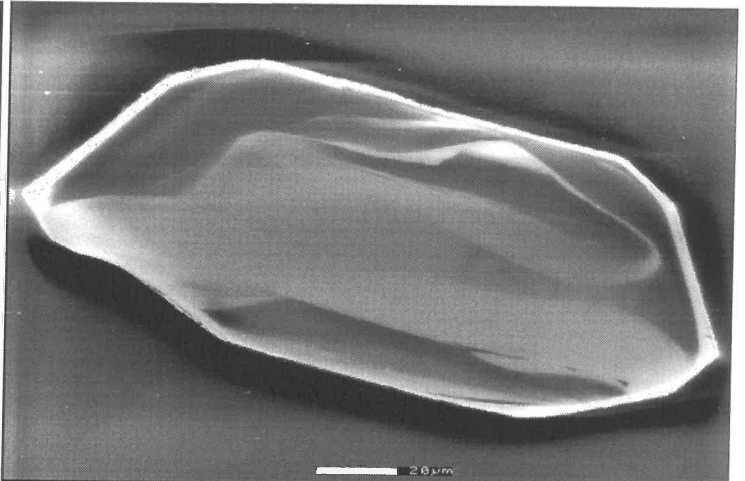


30kV ESD X705 D=10mm P=0.9T
Centre for Microscopy, UWA 981206 11:55 P

9889a22s.tif

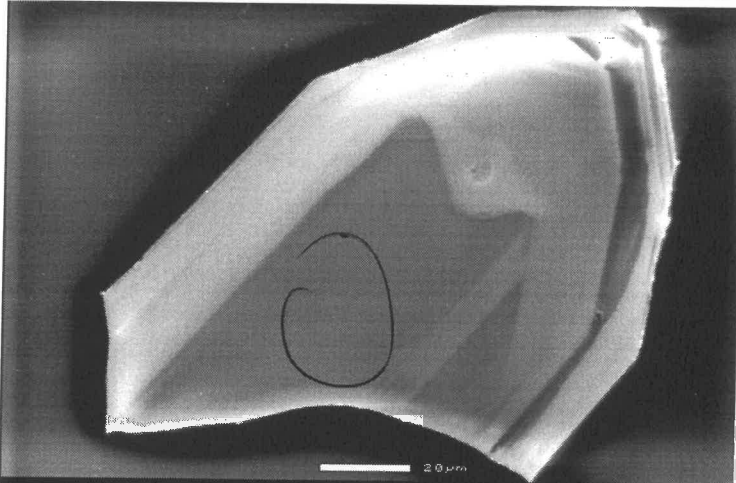


30kV ESD X790 D=10mm P=0.9T
Centre for Microscopy, UWA 981206 12:07 P

9889a23s.tif

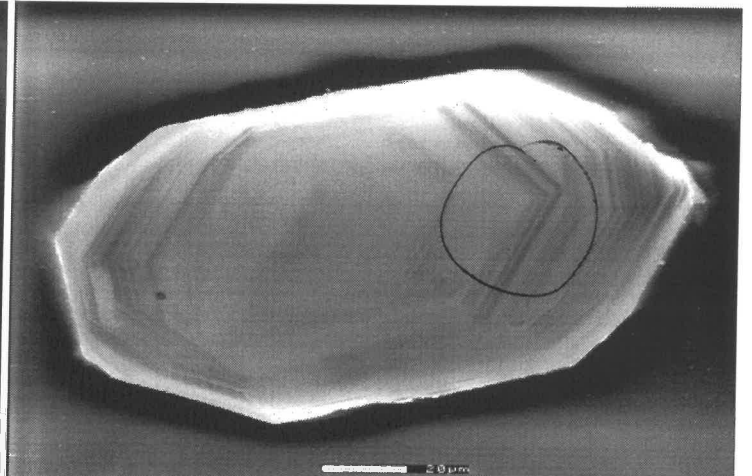


30kV ESD X740 D=9.9mm P=0.9T
Centre for Microscopy, UWA 981206 12:10 P

9889a24s.tif

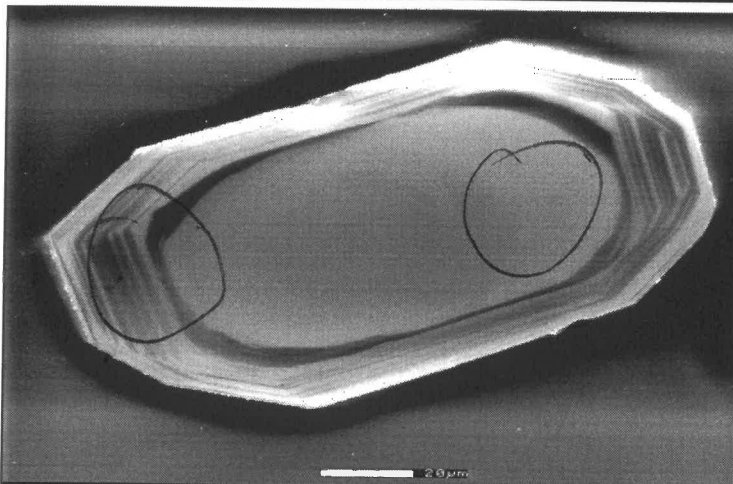


30kV ESD X805 D=9.9mm P=0.9T
Centre for Microscopy, UWA 981206 12:12 P

9889a25s.tif

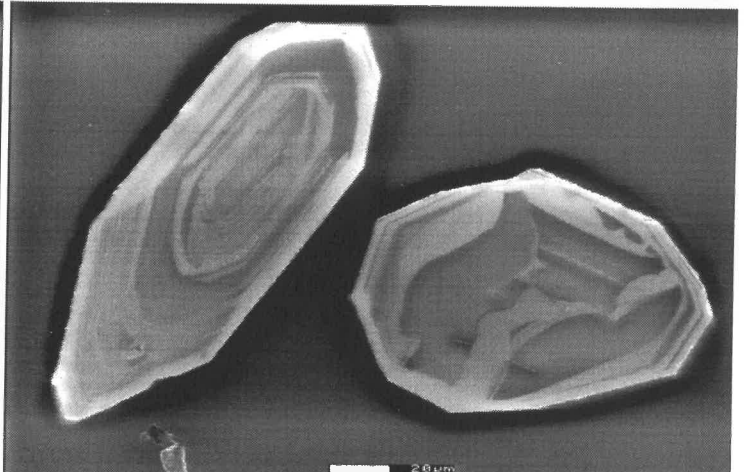


30kV ESD X515 D=9.9mm P=0.9T
Centre for Microscopy, UWA 981206 12:14 P

9889a26s.tif

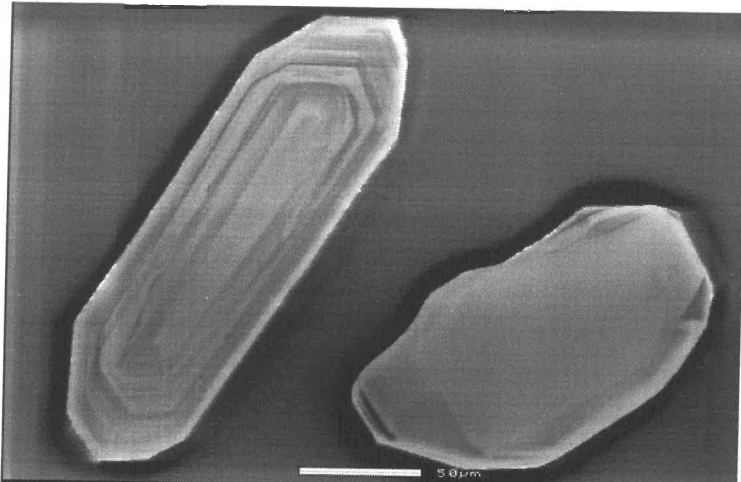


30kV ESD X425 D=9.8mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:16 P

9889a27s.tif

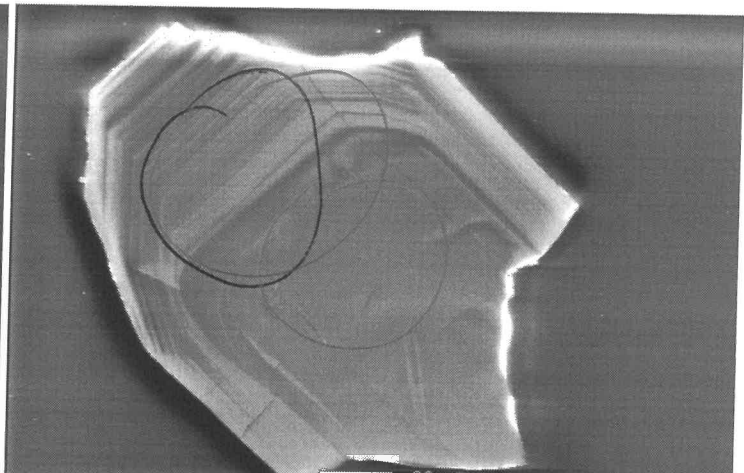


30kV ESD X670 D=9.9mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:19 P

9889a28s.tif

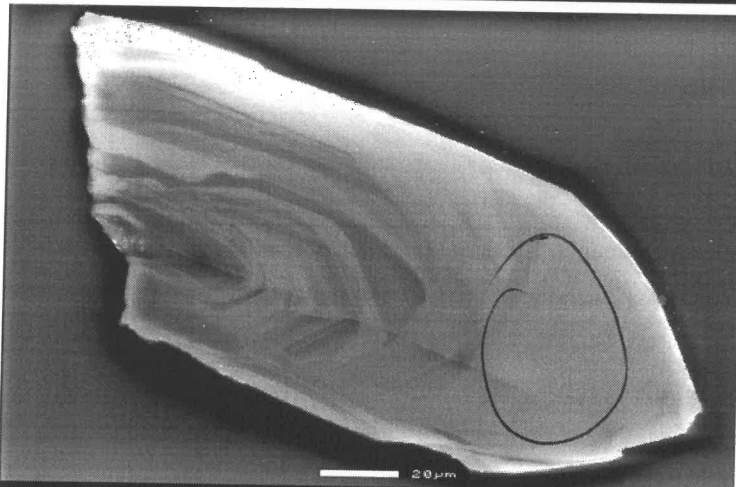


30kV ESD X690 D=9.9mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:21 P

9889a29s.tif

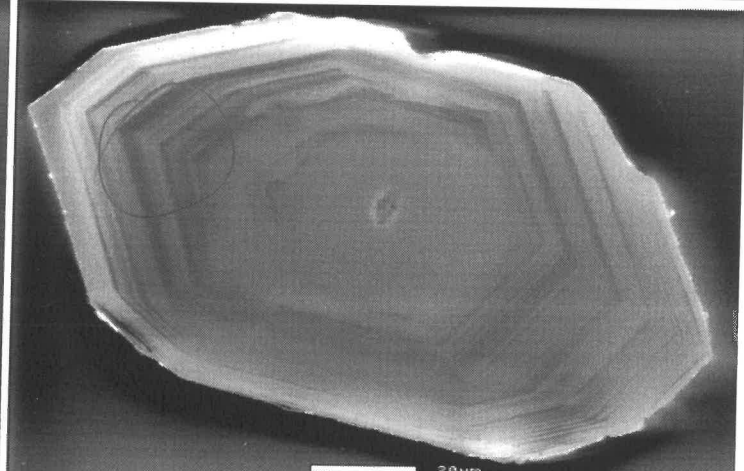


30kV ESD X915 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:24 P

9889a30s.tif

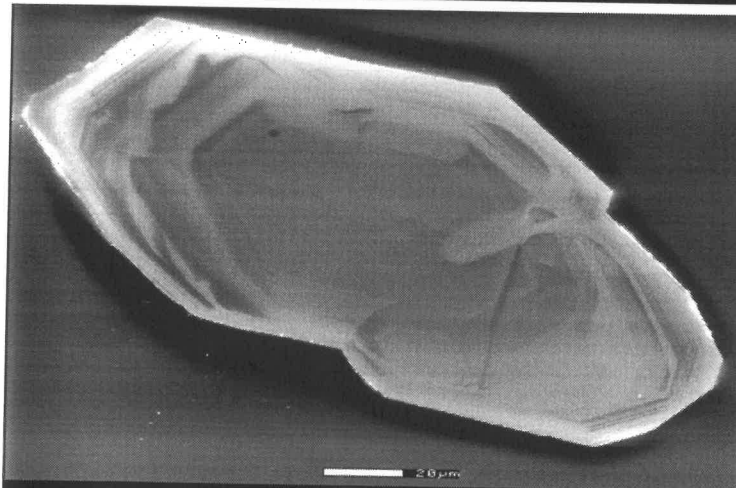


30kV ESD X885 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:27 P

9889a31s.tif

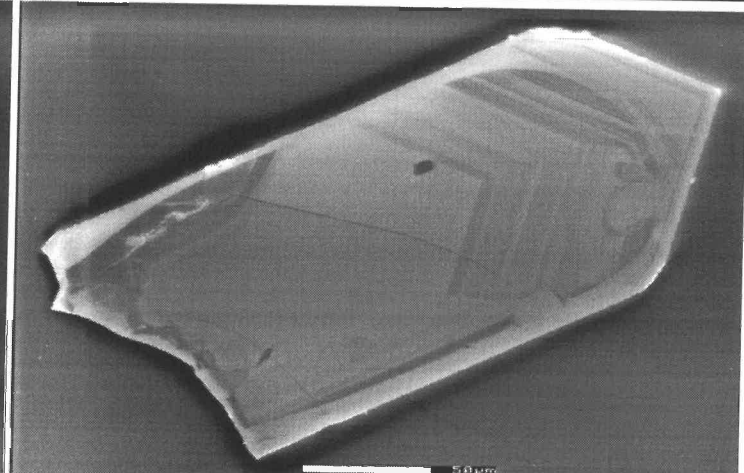


30kV ESD X445 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:29 P

9889a32s.tif

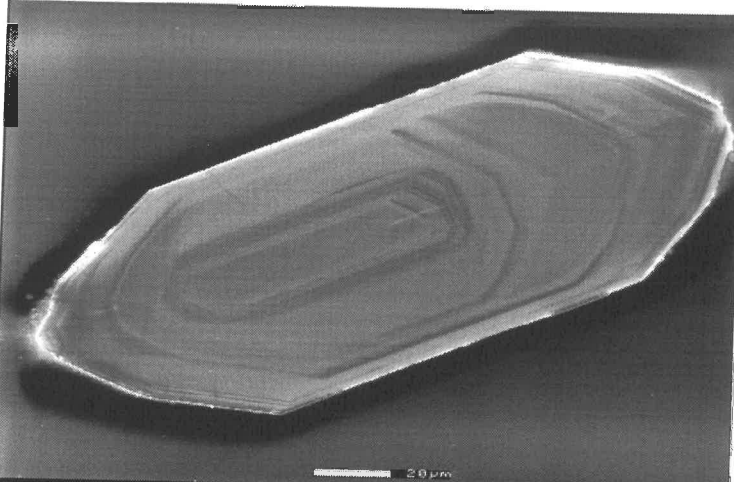


30kV ESD X665 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:31 P

9889a33s.tif

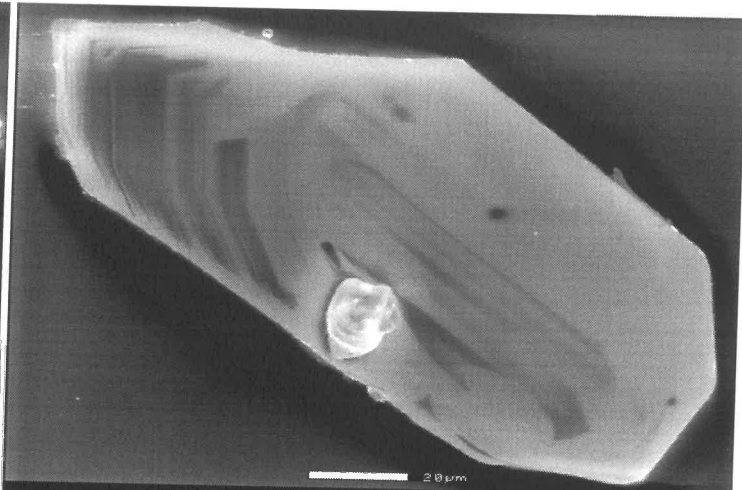

30kV ESD X660 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:33 P

9889a34s.tif

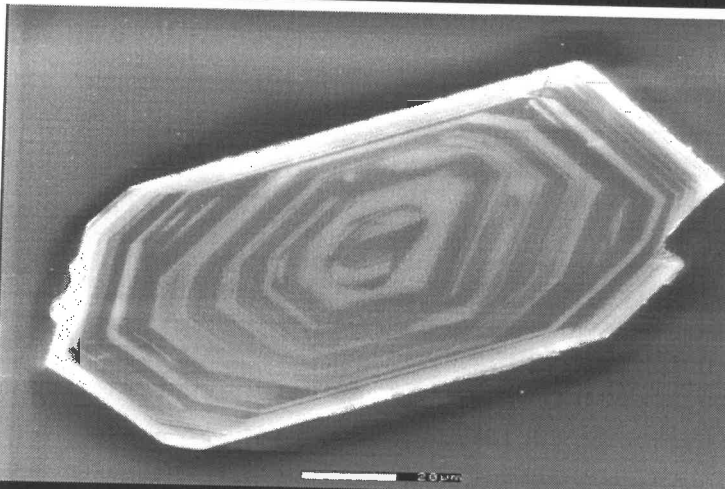

30kV ESD X820 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:35 P

9889a35s.tif



30kV ESD X830 D=10mm P=0.9T
Centre for Microscopy, UWA 98.12.06 12:38 P

9889a36s.tif