



30kV ESD X685 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:01 P

9889c10s.tif

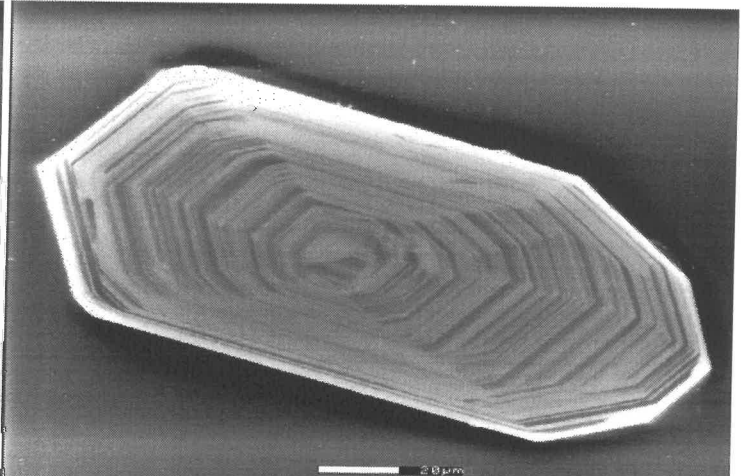


30kV ESD X710 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:04 P

9889c11s.tif

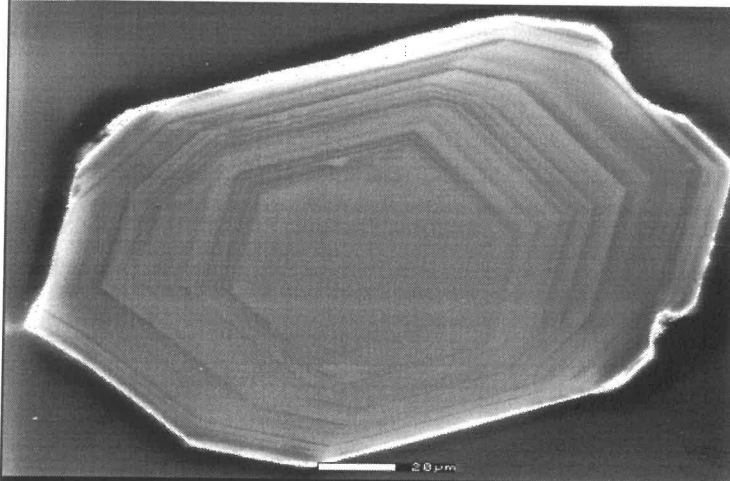


30kV ESD X665 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:06 P

9889c12s.tif

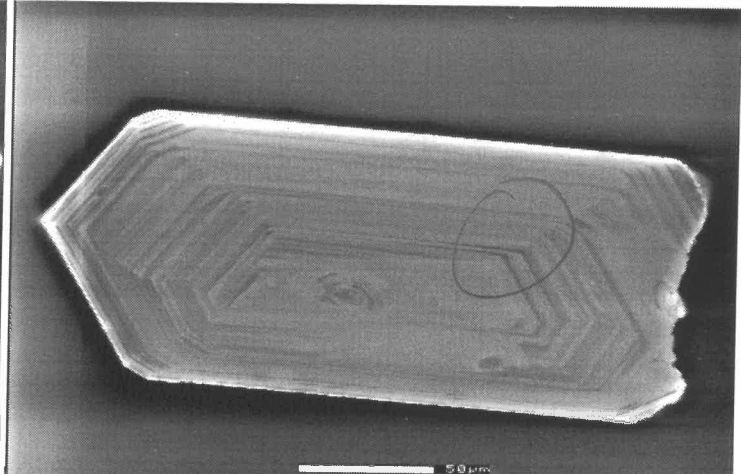


30kV ESD X480 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:06 P

9889c13s.tif

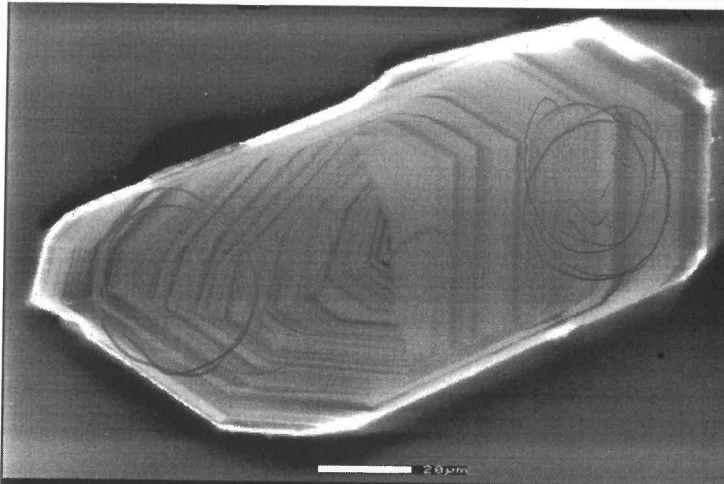


30kV ESD X795 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:10 P

9889c14s.tif

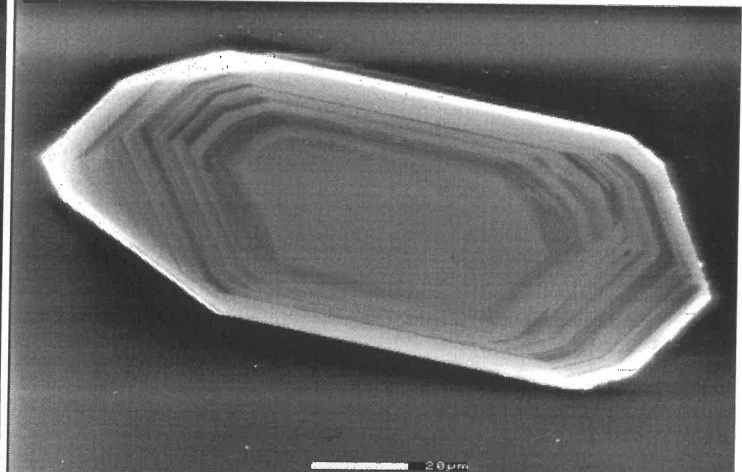


30kV ESD X845 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:12 P

9889c15s.tif

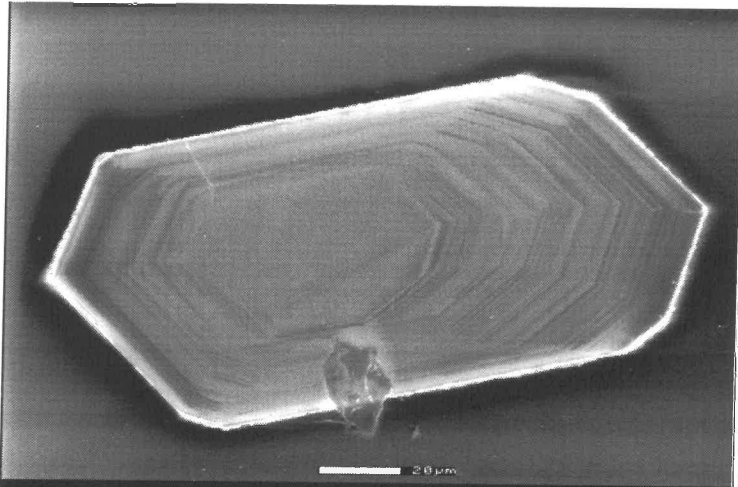


30kV ESD x695 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:14 P

9889c16s.tif

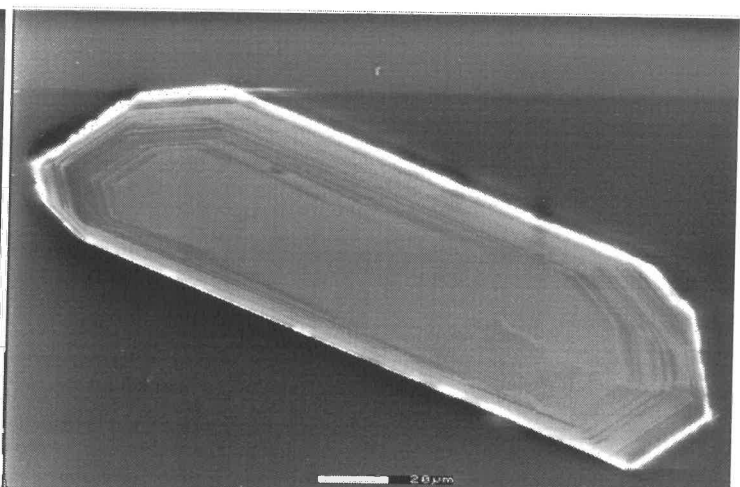


30kV ESD x605 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:16 P

9889c17s.tif

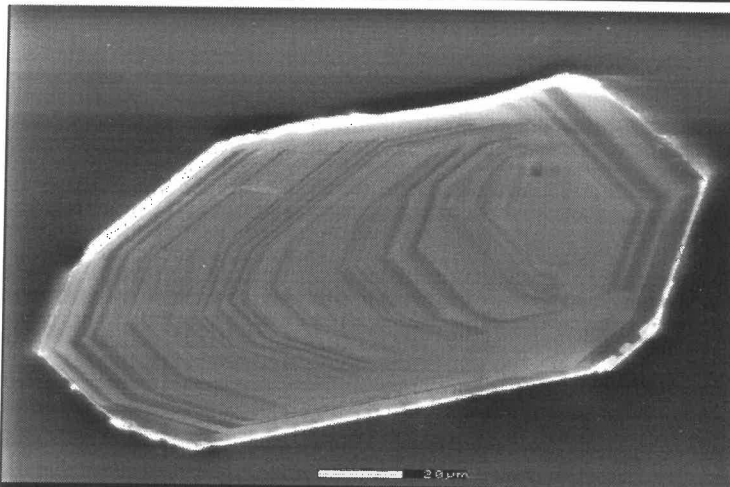


30kV ESD x725 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:19 P

9889c18s.tif

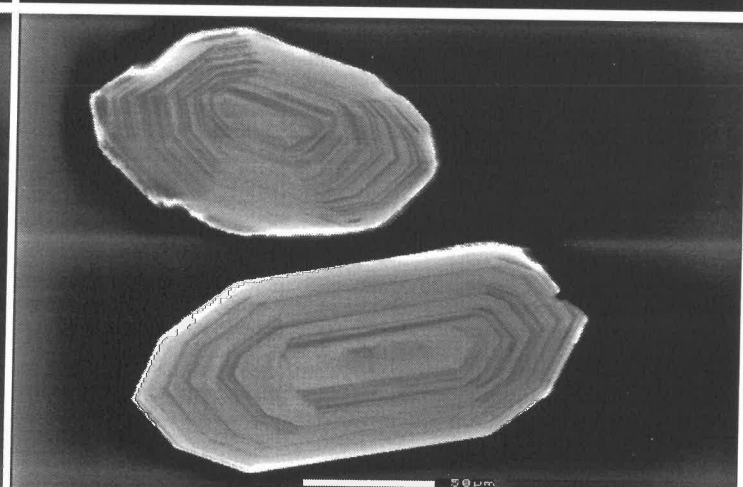


30kV ESD x465 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:21 P

9889c19s.tif

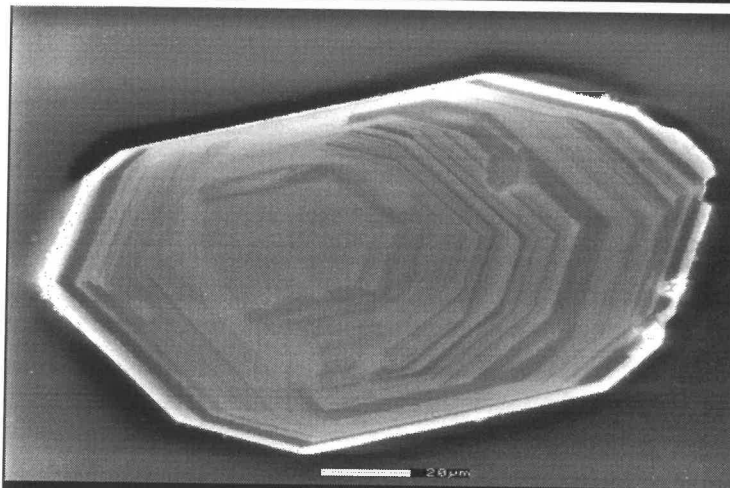


30kV ESD x760 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:22 P

9889c20s.tif

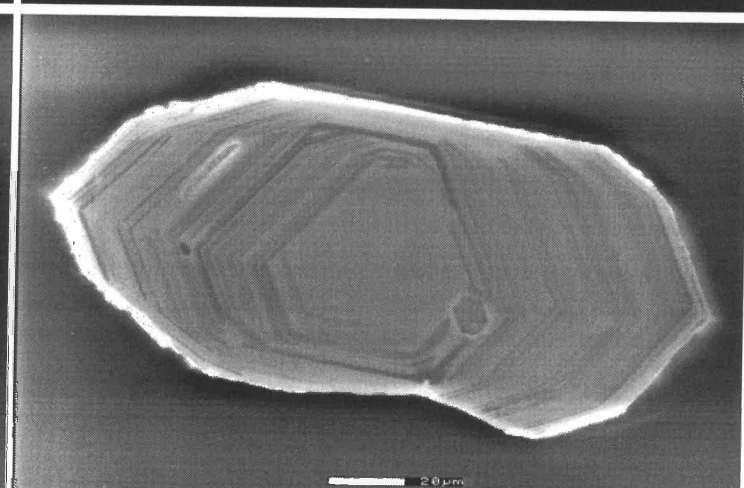


30kV ESD x660 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:25 P

9889c21s.tif

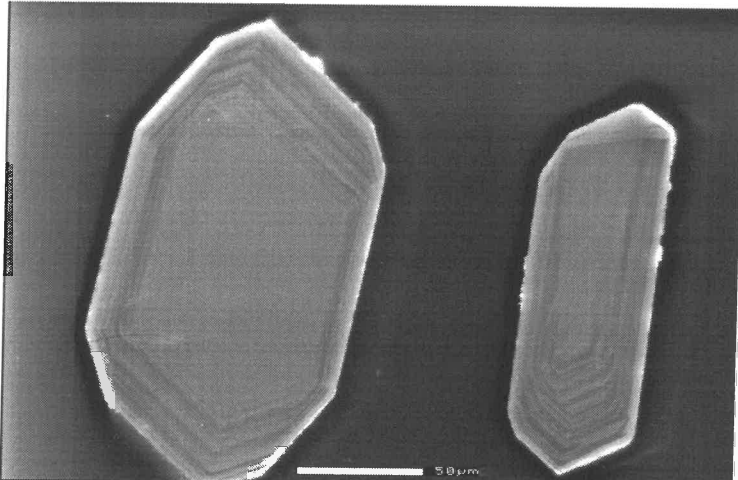


30kV ESD x440 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:27 P

9889c22s.tif

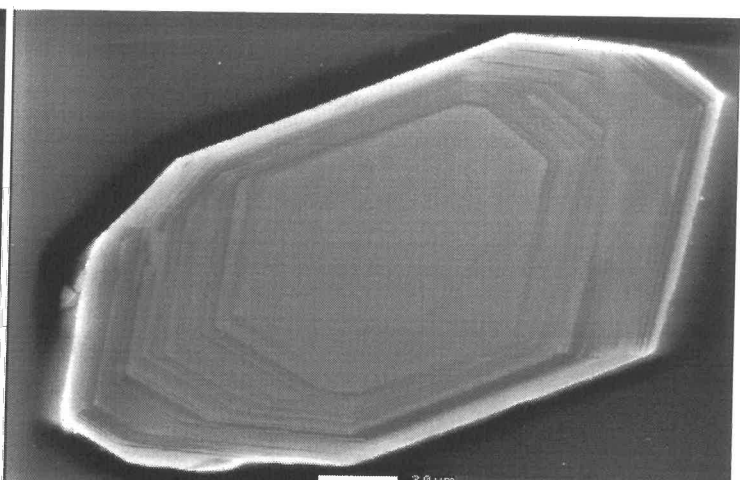


30kV ESD x690 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:29 P

9889c23s.tif

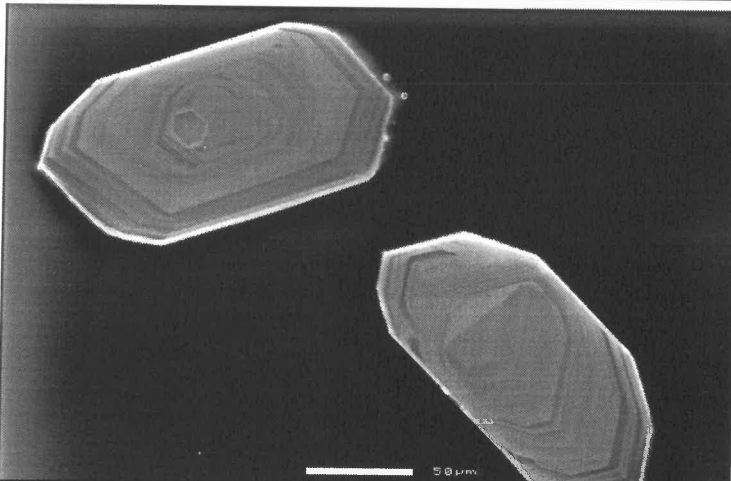


30kV ESD x370 D=9.6mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:32 P

9889c24s.tif

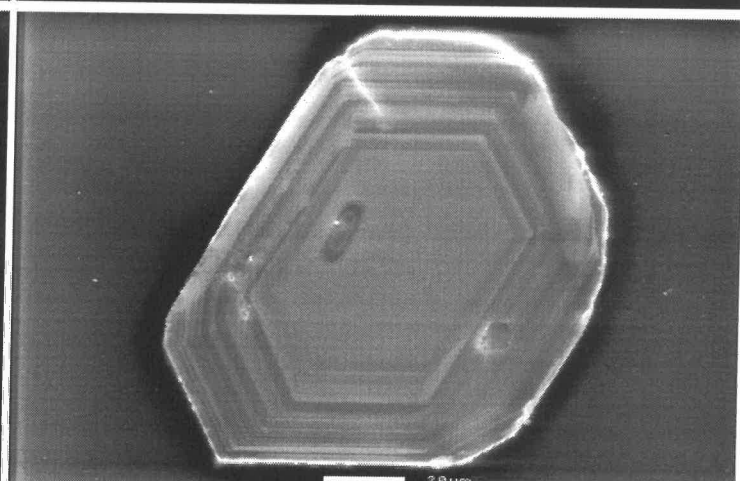


30kV ESD x715 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:34 P

9889c25s.tif

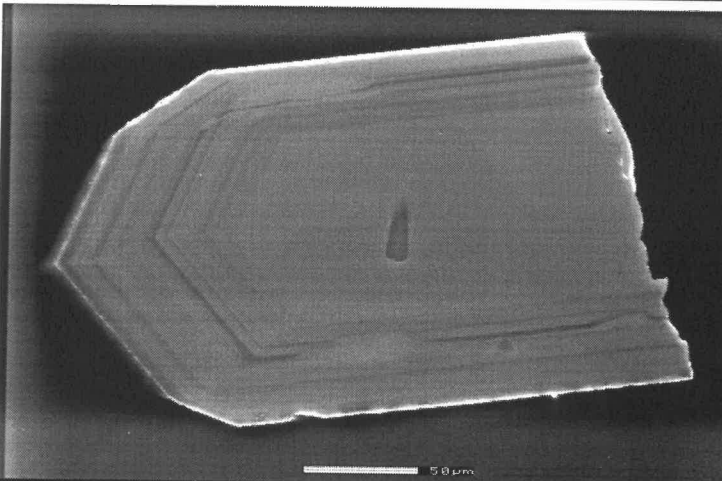


30kV ESD x400 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:38 P

9889c26s.tif

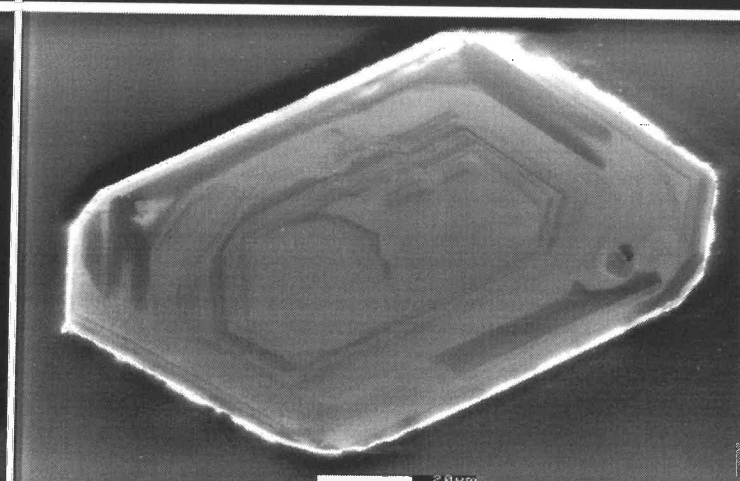


30kV ESD x825 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:38 P

9889c27s.tif

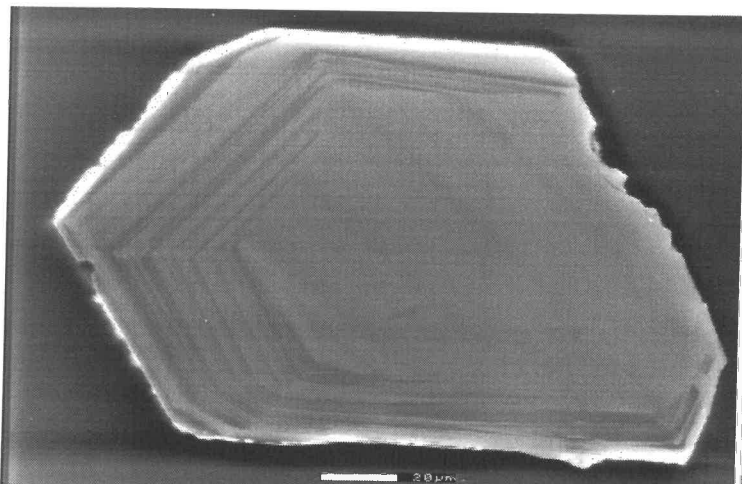


30kV ESD X660 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:45 P

9889c28s.tif

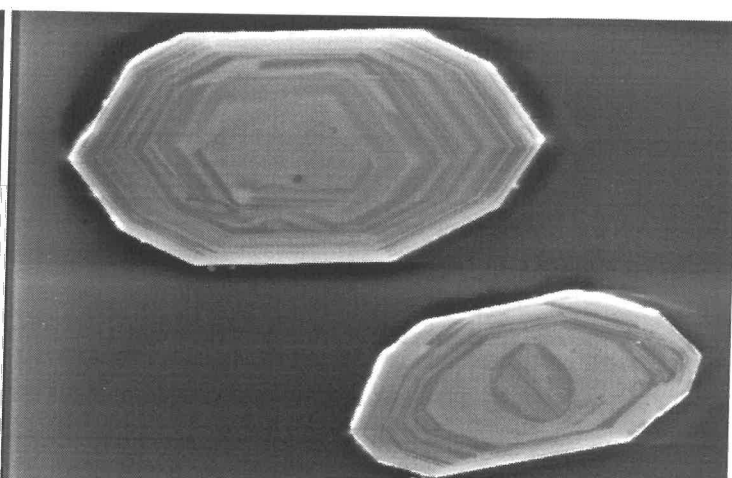


30kV ESD X550 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:43 P

9889c29s.tif

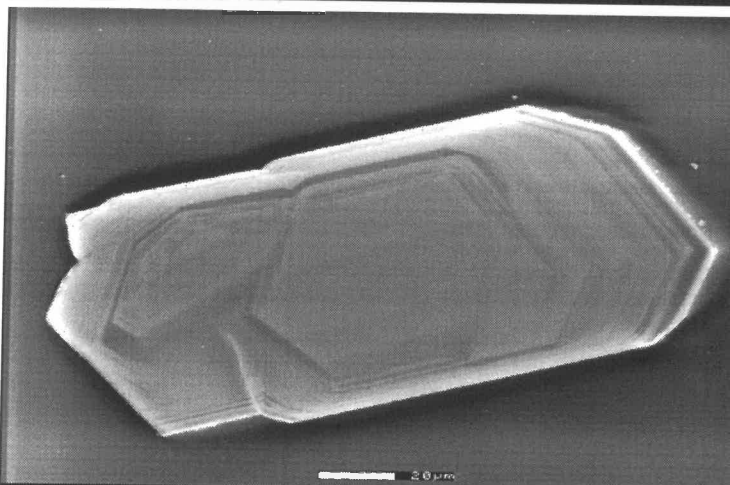


30kV ESD X660 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:45 P

9889c30s.tif

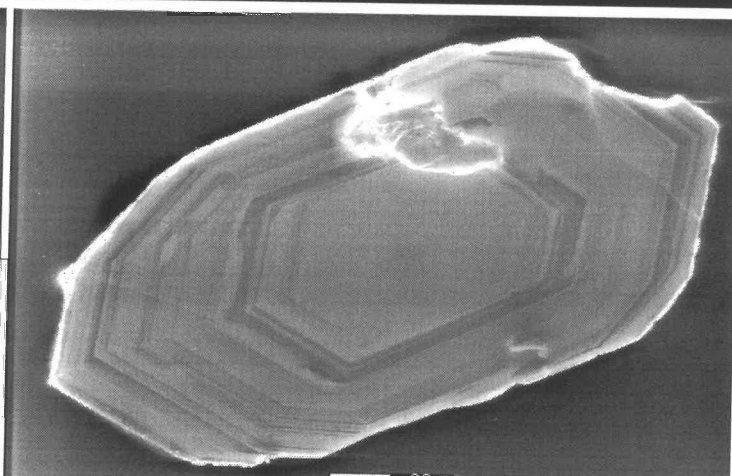


30kV ESD X520 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:47 P

9889c31s.tif

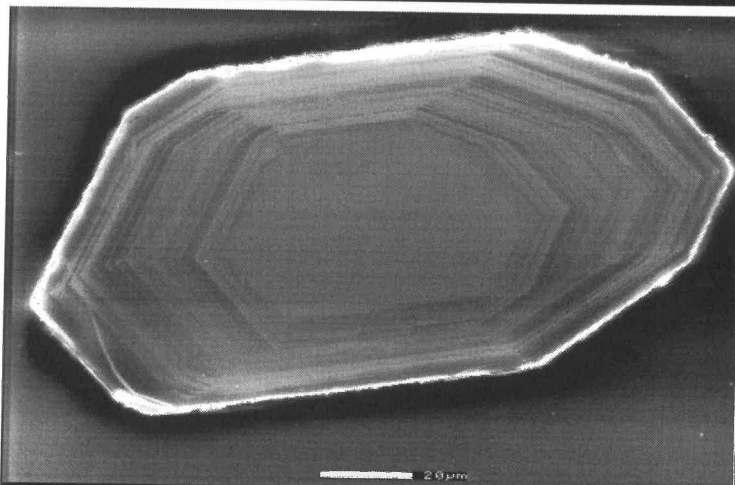


30kV ESD X795 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:49 P

9889c32s.tif

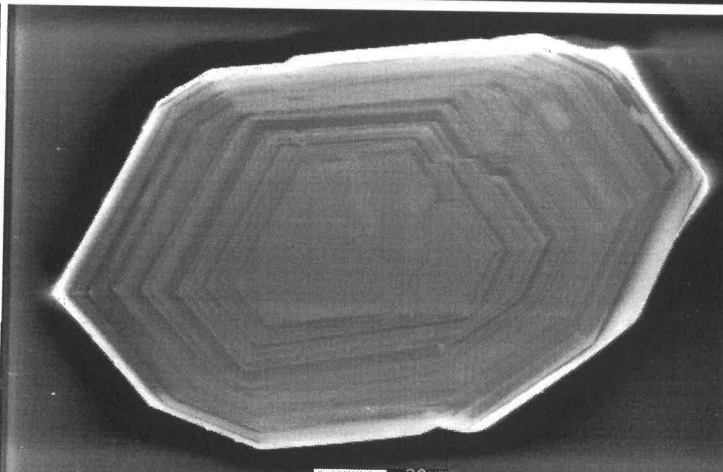


30kV ESD X640 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.98 12:52 P

9889c33s.tif

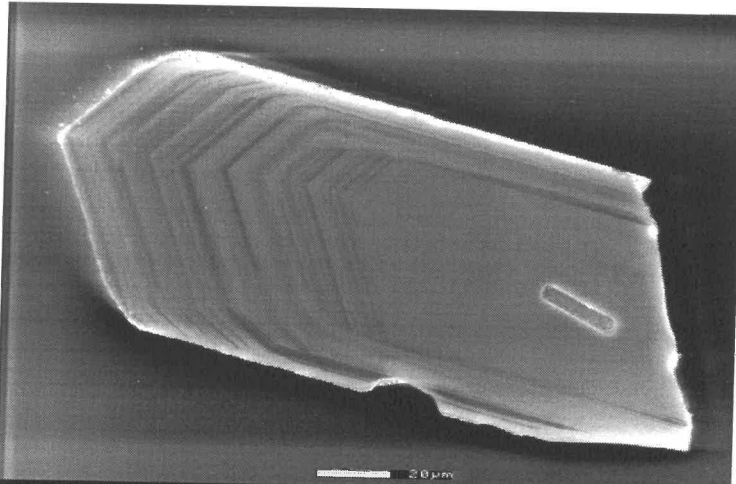


30kV ESD X635 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:54 P

9889c34s.tif

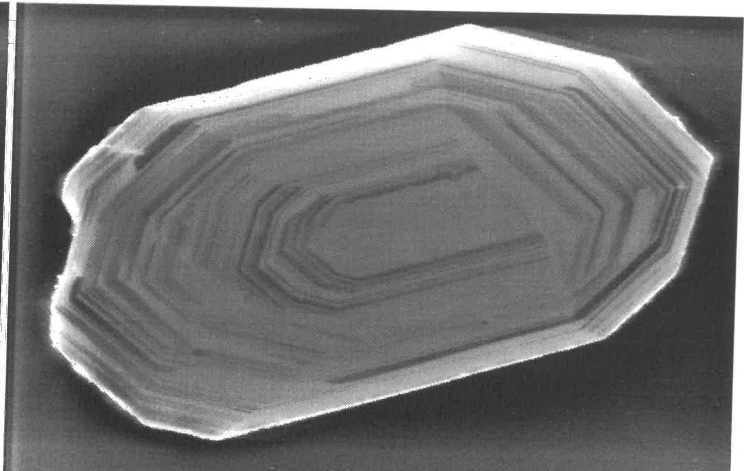

30kV ESD X755 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:56 P

9889c35s.tif

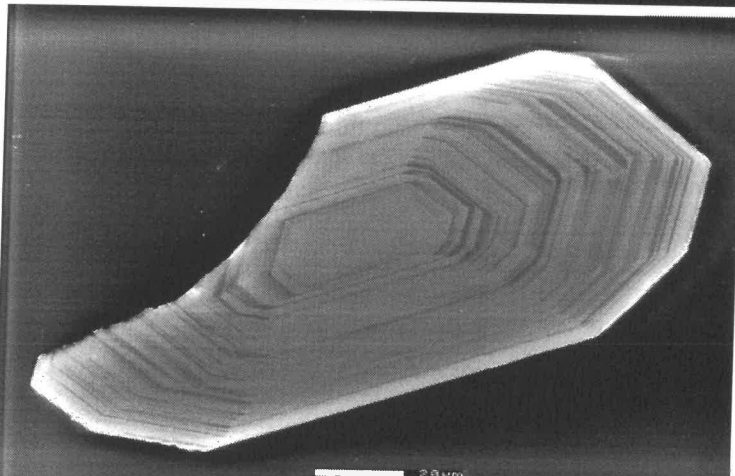

30kV ESD X780 D=9.7mm P=1.3T
Centre for Microscopy, UWA 98.12.08 12:58 P

9889c36s.tif