



30kV ESD X700 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:06 F

9890b04s.tif

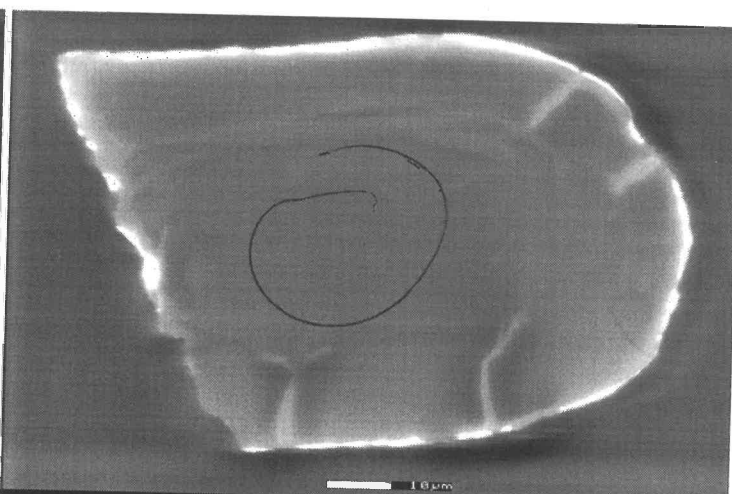


30kV ESD X1100 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:09 F

9890b05s.tif

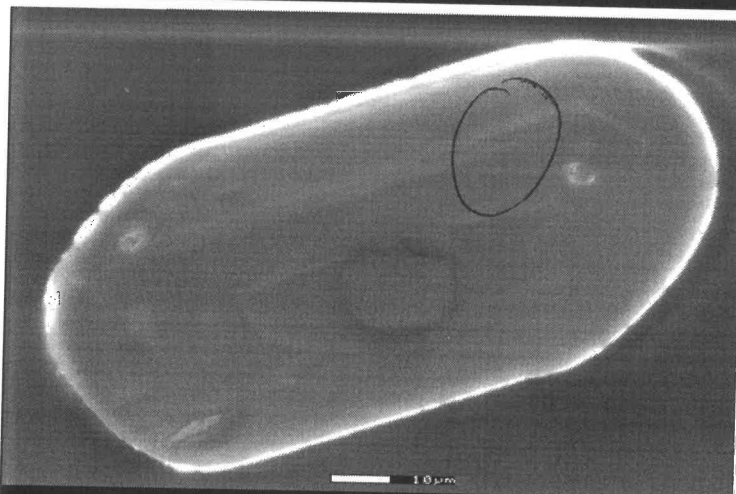


30kV ESD X1000 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:11 P

9890b06s.tif

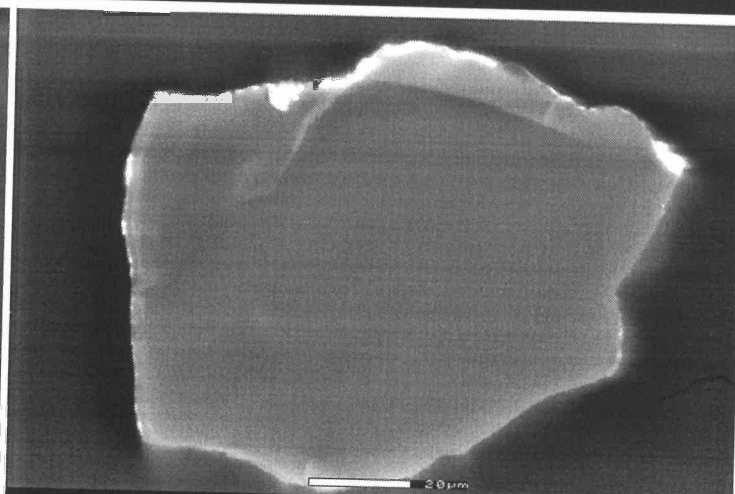


30kV ESD X875 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:14 P

9890b07s.tif

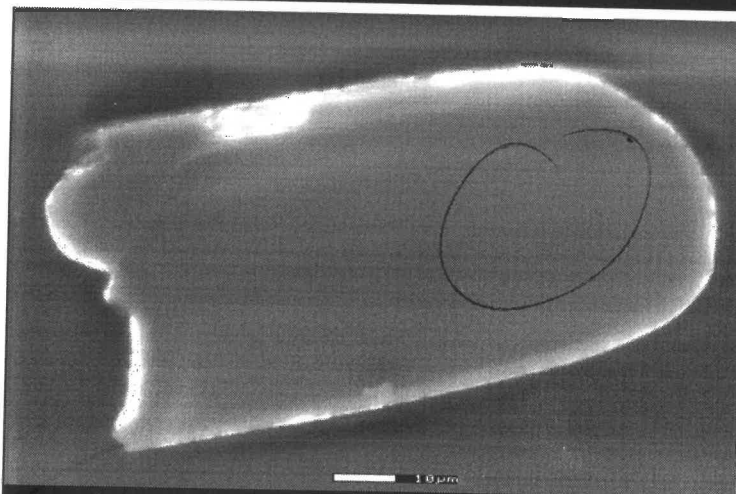


30kV ESD X1100 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:16 P

9890b08s.tif

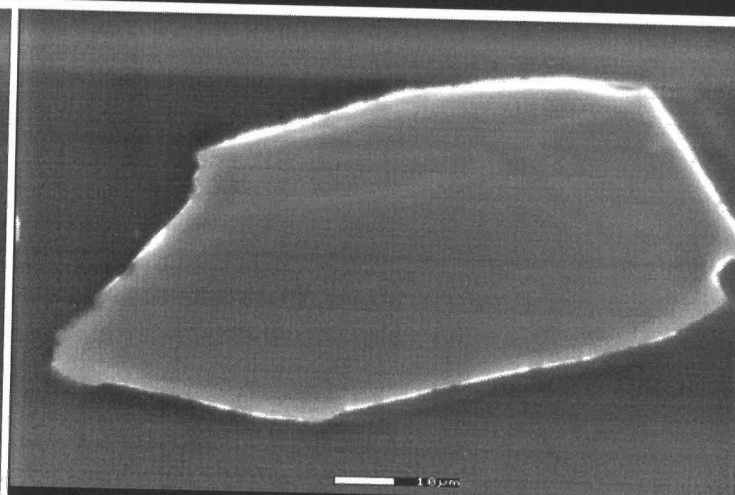


30kV ESD X1000 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:18 P

9890b09s.tif

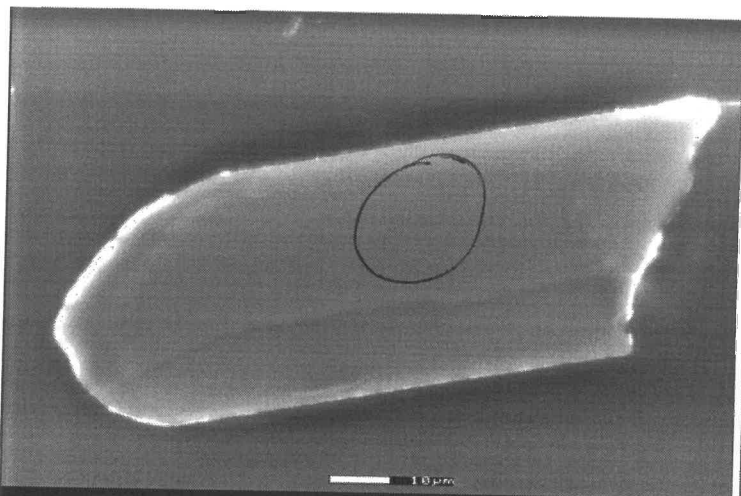


30kV ESD X1050 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:21 P

9890b10s.tif

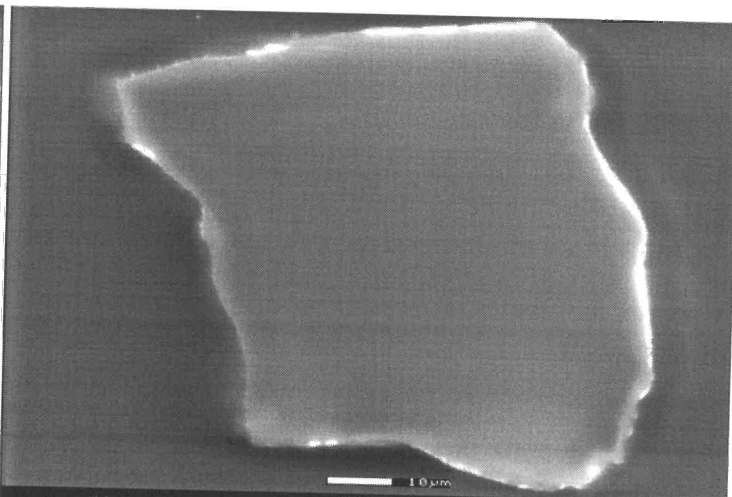


30kV ESD X1150 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:23 P

9890b11s.tif

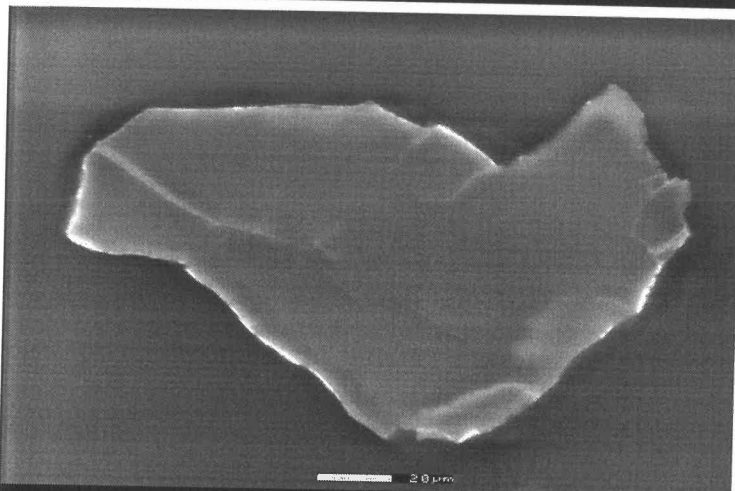


30kV ESD X655 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:25 P

9890b12s.tif

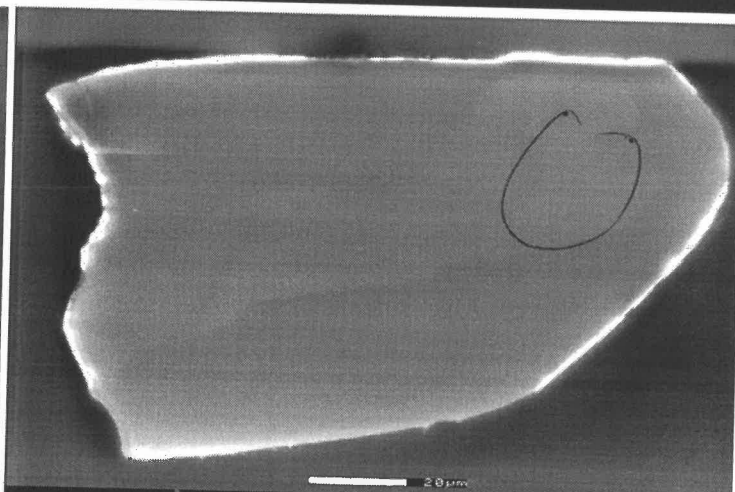


30kV ESD X650 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:28 P

9890b13s.tif

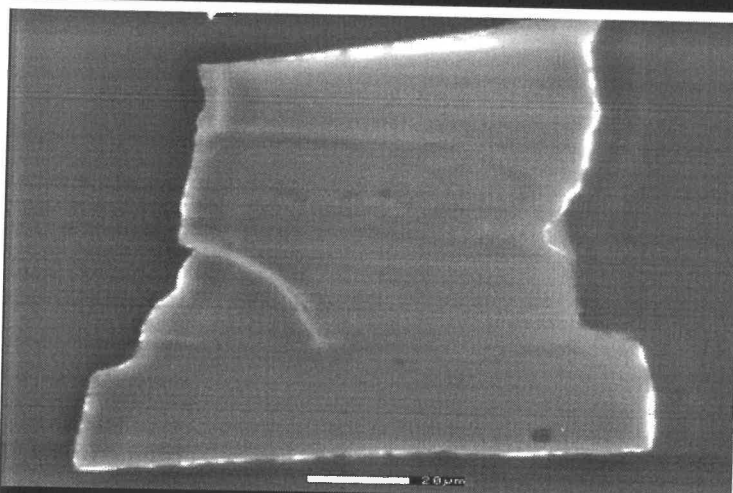


30kV ESD X905 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:31 P

9890b14s.tif

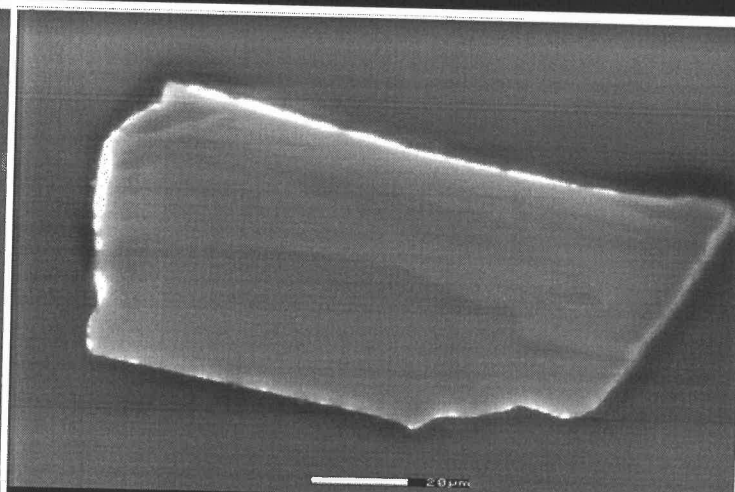


30kV ESD X835 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:33 P

9890b15s.tif

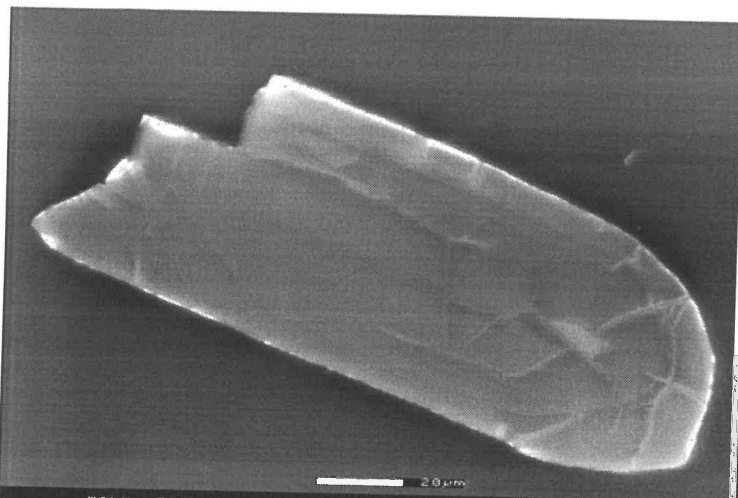


30kV ESD x755 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:37 P

9890b16s.tif

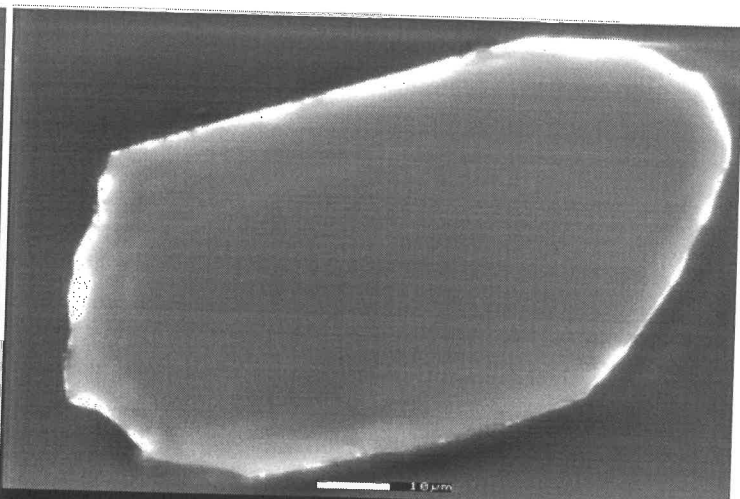


30kV ESD x1300 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:41 P

9890b17s.tif

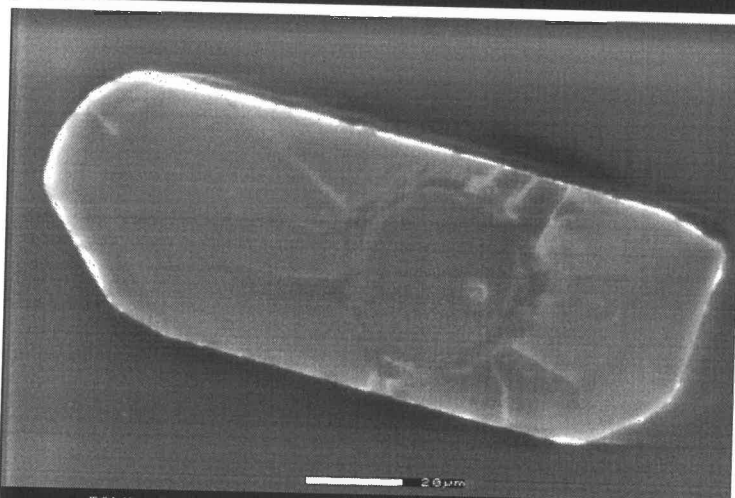


30kV ESD x835 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:43 P

9890b18s.tif

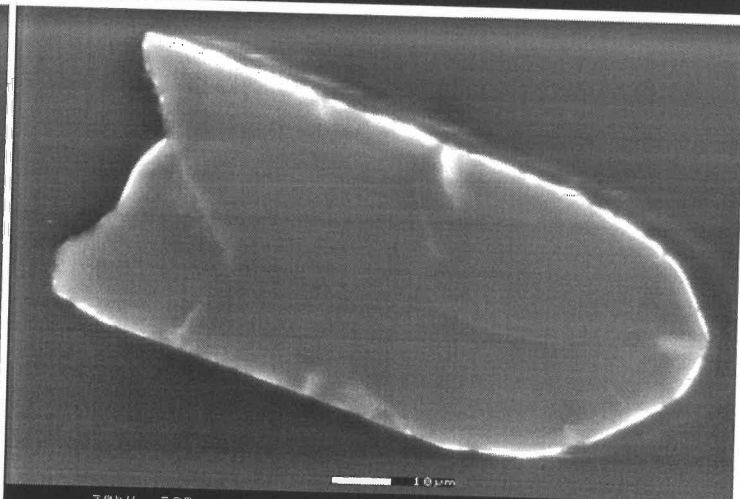


30kV ESD x1000 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:45 P

9890b19s.tif

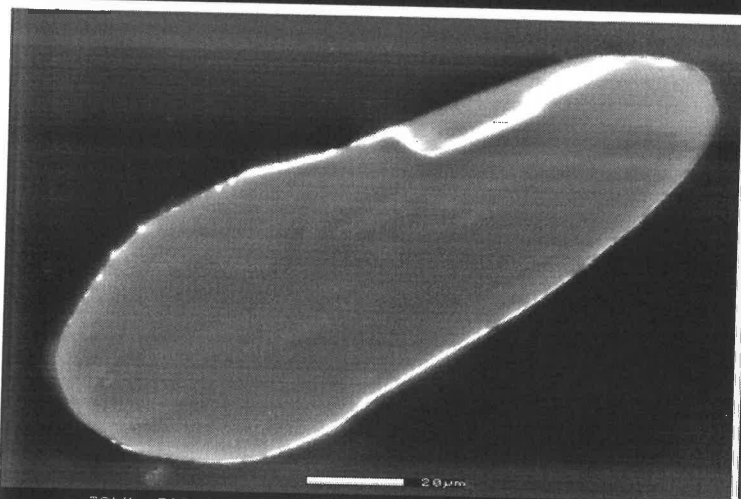


30kV ESD x850 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:48 P

9890b20s.tif

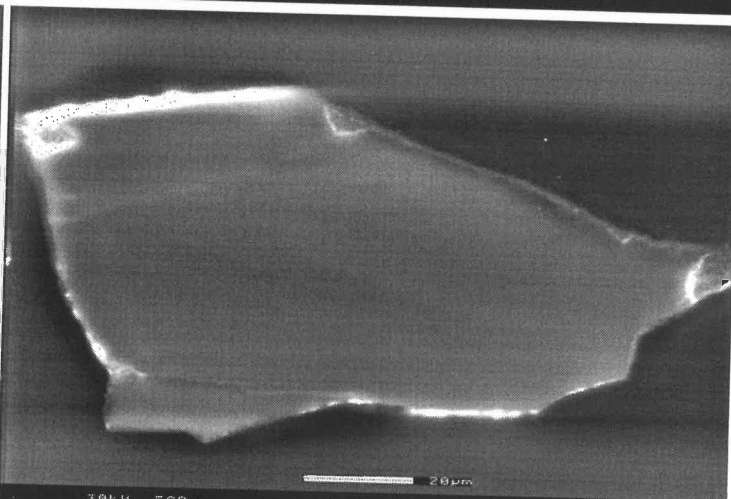


30kV ESD x965 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:52 P

9890b21s.tif

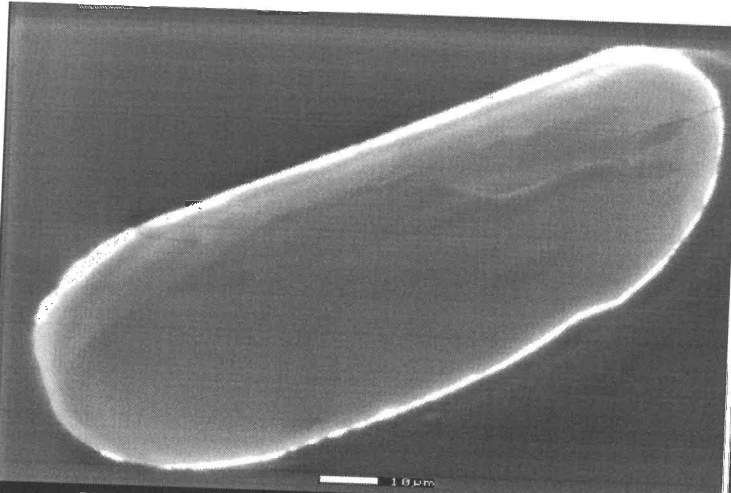


30kV ESD X1000 D=9.9mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:54 P

9890b22s.tif

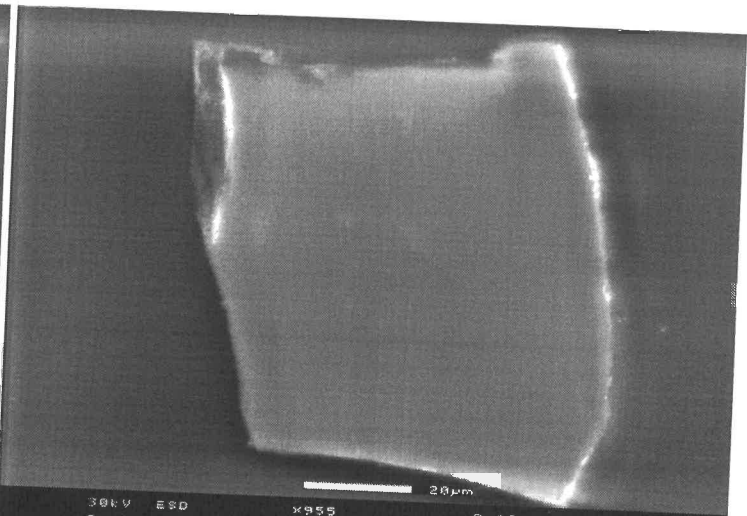


30kV ESD X955 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:57 P

9890b23s.tif

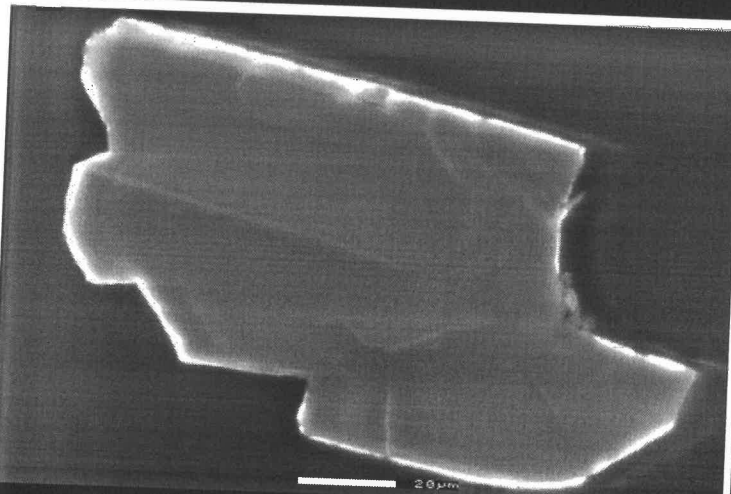


30kV ESD X835 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 22:59 P

9890b24s.tif

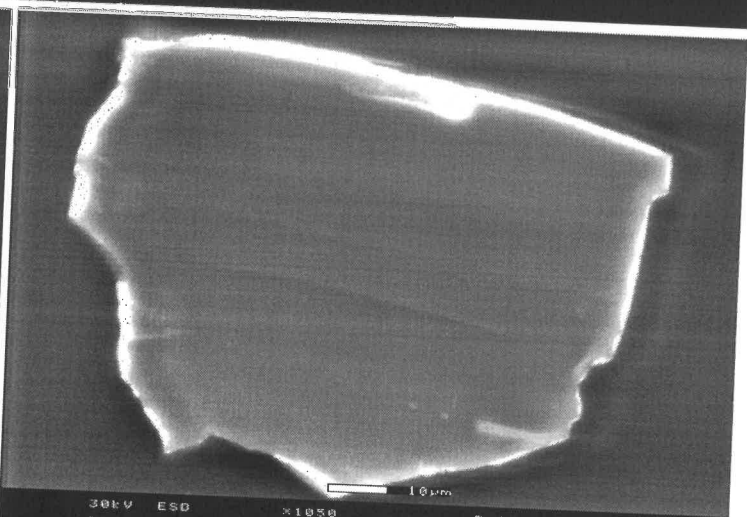


30kV ESD X1050 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 23:02 P

9890b25s.tif

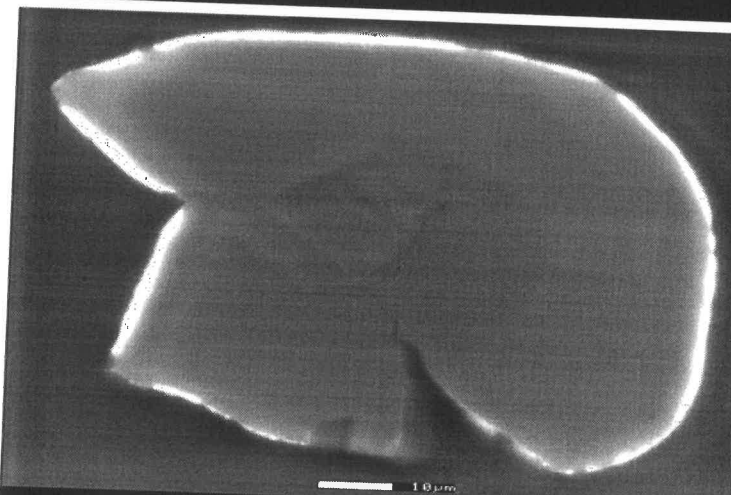

30kV ESD X1250 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 23:05 P

9890b26s.tif

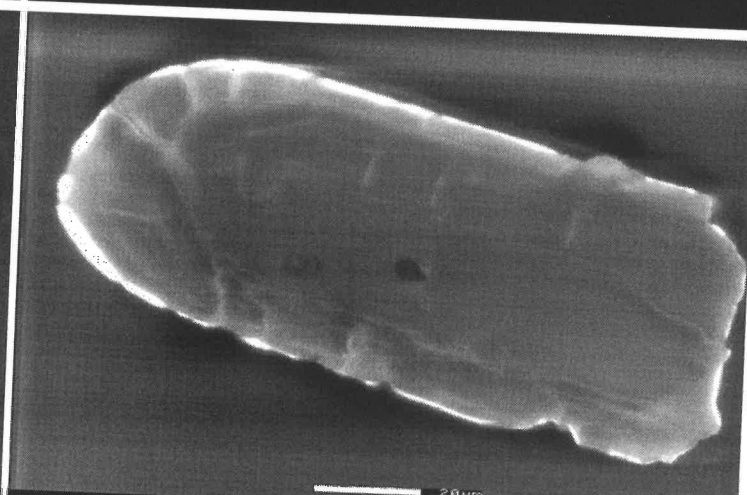

30kV ESD X940 D=10mm P=1.3T  
Centre for Microscopy, UWA 98.12.12 23:10 P

9890b27s.tif